

# Physician's

pocket reference guide

Indications for use

Component ordering information

Introduction system information

Graft specifications


Accessory products

Zenith<sup>®</sup>  
ENDOVASCULAR GRAFTS

Europe



[zenithglobal.cookmedical.com](http://zenithglobal.cookmedical.com)



## Abdominal

Zenith Alpha™ Abdominal (Includes Deployment Overview).....	5
Zenith® Branch (Includes Deployment Overview) .....	21
Zenith Flex® (Includes Deployment Overview) .....	27
Zenith Spiral-Z® .....	39
Zenith Flex® AUI .....	47
Zenith Renu® .....	51

## Fenestrated

Zenith® Fenestrated .....	57
---------------------------	----

## Thoracic

Zenith Alpha™ Thoracic (Includes Deployment Overview) .....	67
Zenith® Dissection.....	85

## Thoracoabdominal

Zenith® t-Branch™ Thoracoabdominal.....	99
---	----

<b>Accessories for endovascular procedures</b> .....	111
Coda® Balloon Catheter .....	112
Lunderquist® Extra-Stiff Wire Guide .....	113
Indy OTW™ Vascular Retriever .....	114
Van Schie Beacon® Tip Seeking Catheter .....	115
Endovascular Dilator Set .....	116
Aurous™ Centimetre Sizing Catheter .....	117
Beacon® Tip Torcon NB® Advantage Catheter .....	118
Beacon® Tip Royal Flush® Plus High-Flow Flush Catheter .....	119
Nester® Embolisation Coils.....	120
Tornado® Embolisation Coils.....	121
Extra-Large Check-Flo® Performer™ Introducer.....	122
Flexor® Keller-Timmermans Introducer .....	123
Flexor® Ansel Check-Flo® Introducer with Hemostasis Valve and High-Flex Dilator.....	124
Performer Introducer.....	126
Amplatz Ultra Stiff Wire Guide.....	127
Roadrunner® UniGlide® Hydrophilic Wire Guide .....	128
Roadrunner® PC Hydrophilic Wire Guide .....	129
Percutaneous Entry Thinwall Needle–One-Part .....	130
Rosen Curved Wire Guide.....	131
<b>Endovascular graft procedure packs</b> .....	133
Zenith Alpha™ Abdominal .....	134
Zenith® AAA.....	135
Zenith® Branch Iliac.....	137
Zenith® Fenestrated .....	138
Zenith Alpha™ Thoracic .....	139
Zenith® TAA.....	140
Zenith® t-Branch .....	141

Please refer to the IFUs for complete instructions. Additional information may be found at [www.cookmedical.com/ai](http://www.cookmedical.com/ai).








Designed to  
help you meet  
the challenges of  
aortic disease.

# Zenith Alpha™

ABDOMINAL ENDOVASCULAR GRAFT

[back](#)

## Indications for use

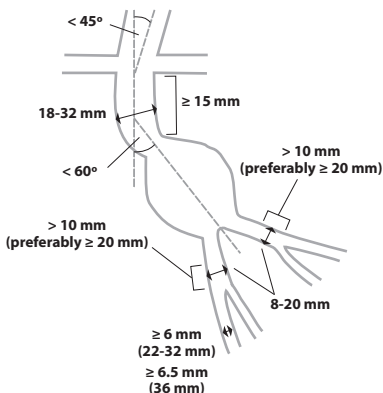

<b>Indications for use</b>	Patients with abdominal aortic or aortoiliac aneurysms having morphology suitable for endovascular repair	
<b>Length</b>	≥ 15 mm nonaneurysmal infrarenal neck	
<b>Aortic fixation site diameter</b>	18-32 mm (measured outer wall to outer wall)	
<b>Angulation/curvature</b>	<ul style="list-style-type: none"> <li>• Angle &lt; 60 degrees relative to the long axis of the aneurysm</li> <li>• Angle &lt; 45 degrees relative to the axis of the suprarenal aorta</li> </ul>	
<b>Ipsilateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 8-20 mm in diameter (measured outer wall to outer wall)	
<b>Contralateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 8-20 mm in diameter (measured outer wall to outer wall)	
<b>Access</b>	Adequate femoral/iliac access compatible with the required introduction systems	
<b>Introducer diameters</b>	22-32 mm grafts: ID 16 Fr (5.3 mm) OD 6.0 mm	36 mm grafts: ID 17 Fr (5.6 mm) OD 6.5 mm
<b>Contraindications</b>	<ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to nitinol, polyester, polypropylene, gold, PTFE, nylon, or urethane</li> <li>• Patients with a systemic infection who may be at increased risk of endovascular graft infection</li> </ul>	

# Bifurcated main body grafts

Order Number	Reference Part Number	Aortic Vessel OD mm	Main Body Diameter mm	Main Body Contralateral Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>					
G35986	ZIMB-22-70	18-19	22	70	16 (5.3)/6.0
G35987	ZIMB-22-84	18-19	22	84	16 (5.3)/6.0
G35988	ZIMB-22-98	18-19	22	98	16 (5.3)/6.0
G35989	ZIMB-22-108	18-19	22	108	16 (5.3)/6.0
G35990	ZIMB-22-118	18-19	22	118	16 (5.3)/6.0
G35991	ZIMB-22-128	18-19	22	128	16 (5.3)/6.0
<b>24 mm Diameter</b>					
G35992	ZIMB-24-70	20-21	24	70	16 (5.3)/6.0
G35993	ZIMB-24-84	20-21	24	84	16 (5.3)/6.0
G35994	ZIMB-24-98	20-21	24	98	16 (5.3)/6.0
G35995	ZIMB-24-108	20-21	24	108	16 (5.3)/6.0
G35996	ZIMB-24-118	20-21	24	118	16 (5.3)/6.0
G35997	ZIMB-24-128	20-21	24	128	16 (5.3)/6.0
<b>26 mm Diameter</b>					
G35998	ZIMB-26-70	22	26	70	16 (5.3)/6.0
G35999	ZIMB-26-84	22	26	84	16 (5.3)/6.0
G36030	ZIMB-26-98	22	26	98	16 (5.3)/6.0
G34381	ZIMB-26-108	22	26	108	16 (5.3)/6.0
G34382	ZIMB-26-118	22	26	118	16 (5.3)/6.0
G34383	ZIMB-26-128	22	26	128	16 (5.3)/6.0
<b>28 mm Diameter</b>					
G34384	ZIMB-28-70	23-24	28	70	16 (5.3)/6.0
G34385	ZIMB-28-84	23-24	28	84	16 (5.3)/6.0
G34386	ZIMB-28-98	23-24	28	98	16 (5.3)/6.0
G34387	ZIMB-28-108	23-24	28	108	16 (5.3)/6.0
G34388	ZIMB-28-118	23-24	28	118	16 (5.3)/6.0
G34389	ZIMB-28-128	23-24	28	128	16 (5.3)/6.0

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Bifurcated main body grafts (continued)


Order Number	Reference Part Number	Aortic Vessel OD mm	Main Body Diameter mm	Main Body Contralateral Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>30 mm Diameter</b>					
G34390	ZIMB-30-70	25-26	30	70	16 (5.3)/6.0
G34391	ZIMB-30-84	25-26	30	84	16 (5.3)/6.0
G34392	ZIMB-30-98	25-26	30	98	16 (5.3)/6.0
G34393	ZIMB-30-108	25-26	30	108	16 (5.3)/6.0
G34394	ZIMB-30-118	25-26	30	118	16 (5.3)/6.0
G34395	ZIMB-30-128	25-26	30	128	16 (5.3)/6.0
<b>32 mm Diameter</b>					
G34396	ZIMB-32-70	27-28	32	70	16 (5.3)/6.0
G34397	ZIMB-32-84	27-28	32	84	16 (5.3)/6.0
G34399	ZIMB-32-98	27-28	32	98	16 (5.3)/6.0
G34400	ZIMB-32-108	27-28	32	108	16 (5.3)/6.0
G34401	ZIMB-32-118	27-28	32	118	16 (5.3)/6.0
G34402	ZIMB-32-128	27-28	32	128	16 (5.3)/6.0
<b>36 mm Diameter</b>					
G34403	ZIMB-36-70	29-32	36	70	17 (5.6)/6.5
G34404	ZIMB-36-84	29-32	36	84	17 (5.6)/6.5
G34405	ZIMB-36-98	29-32	36	98	17 (5.6)/6.5
G34406	ZIMB-36-108	29-32	36	108	17 (5.6)/6.5
G34407	ZIMB-36-118	29-32	36	118	17 (5.6)/6.5
G34408	ZIMB-36-128	29-32	36	128	17 (5.6)/6.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### Introduction system for main body grafts




22-32 mm grafts: 16 Fr (5.3 mm) ID/6.0 mm OD

36 mm grafts: 17 Fr (5.6 mm) ID/6.5 mm OD






# Bifurcated main body grafts

22, 24, 26, 28, 30, 32, 36 mm    22, 24, 26, 28, 30, 32, 36 mm    22, 24, 26, 28, 30, 32, 36 mm



22, 24, 26, 28, 30, 32, 36 mm    22, 24, 26, 28, 30, 32, 36 mm    22, 24, 26, 28, 30, 32, 36 mm




ZIMB-XX-YYY

ZIMB-(main body diameter)-(main body contralateral length)


**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

Designed to  
help you meet  
the challenges of  
aortic disease.



Zenith Alpha™  
SPIRAL-Z® ENDOVASCULAR LEG

## Indications for use



<b>Indications for use</b>	For use with the Zenith® AAA Endovascular Graft family of products, during either a primary or a secondary procedure in patients who have adequate iliac/femoral access compatible with the required introduction systems.	
<b>Ipsilateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 8-20 mm in diameter (measured outer wall to outer wall)	
<b>Contralateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 8-20 mm in diameter (measured outer wall to outer wall)	
<b>Access</b>	Adequate femoral/iliac access compatible with the required introduction systems	
<b>Introducer diameters</b>	9-16 mm grafts: ID 12 Fr (4.0 mm) OD 4.7 mm	20-24 mm grafts: ID 14 Fr (4.7 mm) OD 5.3 mm
<b>Contraindications</b>	<ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to stainless steel, PTFE, polyester, solder (tin, silver), polypropylene, or gold</li> <li>• Patients with a systemic infection who may be at increased risk of endovascular graft infection</li> </ul>	

# Contralateral/ipsilateral iliac leg grafts

Order Number	Reference Part Number	Iliac Leg Distal Diameter mm	Iliac Leg Working Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>9 mm Diameter</b>				
G35955	ZISL-9-42	9	42	12 (4.0)/4.7
G35956	ZISL-9-59	9	59	12 (4.0)/4.7
G35957	ZISL-9-77	9	77	12 (4.0)/4.7
G34508	ZISL-9-93	9	93	12 (4.0)/4.7
G35959	ZISL-9-110	9	110	12 (4.0)/4.7
G35960	ZISL-9-125	9	125	12 (4.0)/4.7
<b>11 mm Diameter</b>				
G35961	ZISL-11-42	11	42	12 (4.0)/4.7
G35962	ZISL-11-59	11	59	12 (4.0)/4.7
G35963	ZISL-11-77	11	77	12 (4.0)/4.7
G35964	ZISL-11-93	11	93	12 (4.0)/4.7
G35965	ZISL-11-110	11	110	12 (4.0)/4.7
G35966	ZISL-11-125	11	125	12 (4.0)/4.7
<b>13 mm Diameter</b>				
G35967	ZISL-13-42	13	42	12 (4.0)/4.7
G35968	ZISL-13-59	13	59	12 (4.0)/4.7
G35969	ZISL-13-77	13	77	12 (4.0)/4.7
G35970	ZISL-13-93	13	93	12 (4.0)/4.7
G34409	ZISL-13-110	13	110	12 (4.0)/4.7
G34410	ZISL-13-125	13	125	12 (4.0)/4.7
<b>16 mm Diameter</b>				
G35971	ZISL-16-42	16	42	12 (4.0)/4.7
G35972	ZISL-16-59	16	59	12 (4.0)/4.7
G35973	ZISL-16-77	16	77	12 (4.0)/4.7
G35975	ZISL-16-93	16	93	12 (4.0)/4.7
<b>20 mm Diameter</b>				
G35977	ZISL-20-42	20	42	14 (4.7)/5.3
G35976	ZISL-20-59	20	59	14 (4.7)/5.3
G35980	ZISL-20-77	20	77	14 (4.7)/5.3
G35981	ZISL-20-93	20	93	14 (4.7)/5.3

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.



## Contralateral/ipsilateral iliac leg grafts (continued)


Order Number	Reference Part Number	Iliac Leg Distal Diameter mm	Iliac Leg Working Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>24 mm Diameter</b>				
G35982	ZISL-24-42	24	42	14 (4.7)/5.3
G35983	ZISL-24-59	24	59	14 (4.7)/5.3
G35984	ZISL-24-77	24	77	14 (4.7)/5.3
G35985	ZISL-24-93	24	93	14 (4.7)/5.3

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.



### Z-Trak® Introduction System for iliac legs

9-16 mm grafts: 12 Fr (4.0 mm) ID/4.7 mm OD

20-24 mm grafts: 14 Fr (4.7 mm) ID/5.3 mm OD



# Contralateral/ipsilateral iliac leg grafts





ZISL-XX-YYY

ZISL-(distal diameter)-(working length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths.

## Contralateral/ipsilateral iliac leg grafts (continued)




ZISL-XX-YYY

ZISL-(distal diameter)-(working length)


**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths.

# Contralateral/ipsilateral iliac leg grafts (continued)

## 20 mm



## 24 mm



# Ancillary components

Order Number	Reference Part Number	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>Main Body Extensions</b>					
G51995	ZLBE-22-45	18-19	22	45	16 (5.3)/6.0
G51997	ZLBE-24-45	20-21	24	45	16 (5.3)/6.0
G51999	ZLBE-26-45	22	26	45	16 (5.3)/6.0
G49290	ZLBE-28-45	23-24	28	45	16 (5.3)/6.0
G52001	ZLBE-30-45	25-26	30	45	16 (5.3)/6.0
G49291	ZLBE-32-45	27-28	32	45	16 (5.3)/6.0
G53387	ZLBE-36-45	29-32	36	45	17 (5.6)/6.5
G51996	ZLBE-22-58	18-19	22	58	16 (5.3)/6.0
G51998	ZLBE-24-58	20-21	24	58	16 (5.3)/6.0
G52000	ZLBE-26-58	22	26	58	16 (5.3)/6.0
G48604	ZLBE-28-58	23-24	28	58	16 (5.3)/6.0
G52002	ZLBE-30-58	25-26	30	58	16 (5.3)/6.0
G48603	ZLBE-32-58	27-28	32	58	16 (5.3)/6.0
G53388	ZLBE-36-58	29-32	36	58	17 (5.6)/6.5


Order Number	Reference Part Number	Main Body Diameter mm	Proximal Diameter mm	Distal Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>Converters</b>						
G52003	ZLC-24-66	22, 24	24	12	66	16 (5.3)/6.0
G48601	ZLC-28-66	26, 28	28	12	66	16 (5.3)/6.0
G48602	ZLC-32-66	30, 32	32	12	66	16 (5.3)/6.0
G53389	ZLC-36-66	36	36	12	66	17 (5.6)/6.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## H&L-B One-Shot® Introduction System for ancillary components

22-32 mm grafts: 16 Fr (5.3 mm) ID/6.0 mm OD


36 mm grafts: 17 Fr (5.6 mm) ID/6.5 mm OD




# Ancillary components

## Main body extensions

22, 24, 26, 28, 30, 32, 36 mm




22, 24, 26, 28, 30, 32, 36 mm



## Converters

24, 28, 32, 36 mm



Main body extensions

ZLBE-XX-YY

ZLBE-(diameter)-(length)

Converters

ZLC-XX-YY

ZLC-(proximal diameter)-(length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths.

# Deployment overview\*

## 1a MAIN BODY PLACEMENT

**Note:** Before insertion, position the main body delivery system on the patient's abdomen under fluoroscopy to determine the orientation of the contralateral limb radiopaque marker.

Insert the main body delivery system over the wire and into the femoral artery. Advance the delivery system until the four gold radiopaque markers (which are positioned 2 mm from the most proximal segment of the graft material) are just inferior to the most inferior renal orifice.

- 1b Stabilize the grey positioner (the shaft of the delivery system) while withdrawing the sheath. Deploy the first two covered stents by withdrawing the sheath while monitoring the device location. Check the position of the contralateral limb radiopaque marker and the location of renal arteries. Continue withdrawing the sheath until the contralateral limb is fully deployed. Stop withdrawing the sheath.

## 2 MAIN BODY PROXIMAL (TOP) DEPLOYMENT

While holding the black gripper, turn the black safety lock knob 180 degrees in the direction of the arrows (counterclockwise). To release the suprarenal bare stent, turn the blue rotation handle approximately two full rotations in the direction of the arrow (clockwise) until a stop is felt.

**Note:** Once you deploy the barbed suprarenal stent, do not reposition the graft.

## 3 CONTRALATERAL ILIAC WIRE GUIDE PLACEMENT

Manipulate wire guide using an angiographic catheter through the open end of the contralateral limb into the body of the graft. Advance the wire guide inside the body of the graft and into the thoracic aorta. AP and oblique fluoroscopic views can aid in verification of device cannulation.

## 4 CONTRALATERAL ILIAC LEG PLACEMENT AND DEPLOYMENT

Remove the femoral sheath and introduce the contralateral iliac leg delivery system into the artery. Advance slowly until the zone between the two proximal gold markers aligns with the gold radiopaque marker at the bifurcation of the main body graft. This will allow between 16 mm and 32 mm of overlap between components.

Confirm position of the distal end of the contralateral iliac leg graft. Reposition the contralateral iliac leg graft if necessary to ensure both internal iliac patency and minimum overlap of 2 stents (16 mm) within the main body endovascular graft. To deploy, hold the contralateral iliac leg graft in position with the grey positioner while withdrawing the sheath approximately 10 mm. Check the graft position and reposition the graft if necessary. Continue to deploy the graft by withdrawing the sheath while continuously checking the graft position. Stop withdrawing the sheath as soon as the distal end of the contralateral iliac leg graft is released. Under fluoroscopy and after verification of the iliac leg graft position, loosen the pin vise and retract the inner cannula to dock the tapered dilator to the grey positioner. Tighten the pin vise. Maintain the sheath position while withdrawing the grey positioner with the secured inner cannula.

## 5 MAIN BODY DISTAL (BOTTOM) DEPLOYMENT

Fully deploy the ipsilateral limb of the main body by withdrawing the sheath until the most distal stent has expanded. Stop withdrawing the sheath.

**Note:** The distal stent is still secured to the delivery system.

While holding the black gripper, turn the grey safety lock knob counterclockwise to engage the blue rotation handle. To release the wire securing the ipsilateral limb to the delivery system, turn the blue rotation handle in the direction of the arrow (clockwise) until a stop is felt. Withdraw the entire inner subassembly through the sheath by holding the Captor Hemostatic Valve stationary and pulling on the black gripper. Confirm that the Captor sleeve is removed along with the inner sub assembly.

**Note:** Maintain the position of the sheath and the wire guide.

Close the Captor Hemostatic Valve on the introducer sheath by turning it in a clockwise direction until it stops.

## Deployment overview\* (continued)

### 6 IPSILATERAL ILIAC LEG PLACEMENT AND DEPLOYMENT

Utilize the main body graft wire and sheath assembly to introduce the ipsilateral iliac leg graft. Advance the dilator and sheath assembly into the main body sheath. Continue advancing it slowly until the proximal edge of the ipsilateral leg graft aligns with the proximal edge of the previously placed contralateral leg graft. Confirm the position of the distal end of the iliac leg graft. Reposition the iliac leg graft, if necessary, to ensure internal iliac patency. To deploy, hold the iliac leg graft in position with the grey positioner while withdrawing the sheath approximately 10 mm. Check the graft position and reposition if necessary. Continue to deploy the graft by withdrawing the sheath while continuously checking the position of the graft. Under fluoroscopy and after you verify the iliac leg graft position, loosen the pin vise and retract the inner cannula to dock the tapered dilator to the positioner. Tighten the pin vise. Maintain the sheath position while using the secured inner cannula to withdraw the grey positioner. Close the Captor Hemostatic Valve by turning it in a clockwise direction until it stops.

### 7 MOLDING BALLOON INSERTION

Advance the molding balloon over the wire guide and through the hemostatic valve of the main body introduction system to the level of the renal arteries. Maintain proper sheath positioning. Tighten the Captor Hemostatic Valve around the molding balloon by turning it clockwise with gentle pressure.

**CAUTION: Do not inflate the balloon in the vessel outside of the graft.**

Expand the molding balloon with diluted contrast media (as directed by the manufacturer) in the area of the most proximal covered stent and the infrarenal neck, starting proximally and working in the distal direction.

**CAUTION: Before you reposition the balloon, confirm that it is completely deflated.**

**CAUTION: The Captor Hemostatic Valve must be open before you reposition the molding balloon.**

Withdraw the molding balloon to the ipsilateral limb overlap region and expand the balloon.

**CAUTION: The Captor Hemostatic Valve must be open before you reposition the molding balloon.**

Withdraw the molding balloon to the ipsilateral distal fixation site and expand the balloon.

**CAUTION: Do not inflate the balloon in the vessel outside of the graft.**

Deflate and remove the molding balloon. Transfer the molding balloon onto the contralateral wire guide and into the contralateral iliac leg introduction system. Advance the molding balloon to the contralateral limb overlap region and expand the balloon.

**CAUTION: Before you reposition the balloon, confirm that it is completely deflated.**

Withdraw the molding balloon to the contralateral iliac leg distal fixation site and expand the balloon.


**CAUTION: Do not inflate the balloon in the vessel outside of the graft.**

Remove the molding balloon and replace it with an angiographic catheter to perform completion angiography.

Remove or replace all stiff wire guides to allow the iliac arteries to resume their natural position.

*\*This deployment overview is an outline highlighting the deployment process for the Zenith Alpha Abdominal Endovascular Graft. The Instructions for Use booklet should be consulted for a more thorough examination of the deployment protocol, indications, contraindications, warnings, and precautions.*



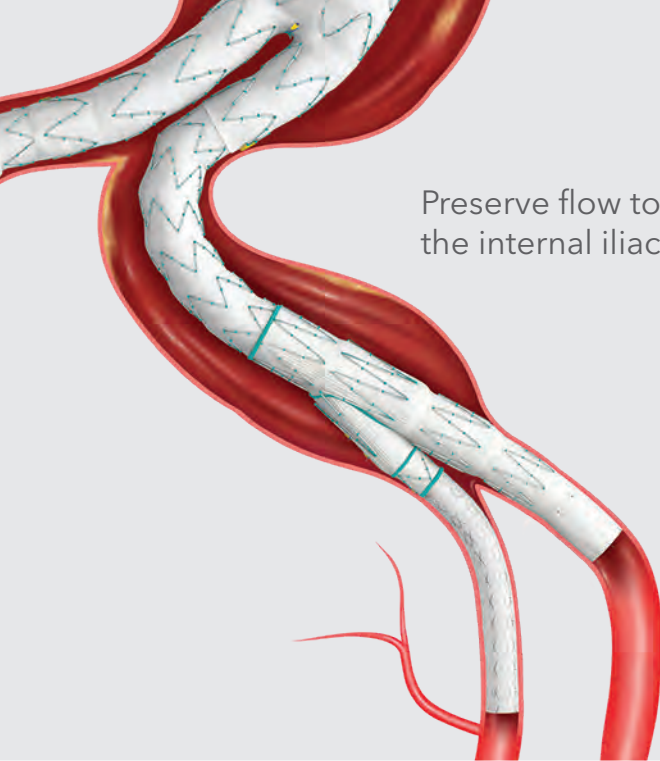


Preserve flow to  
the internal iliacs.

# Zenith<sup>®</sup> Branch

ILIAC ENDOVASCULAR GRAFT

[back](#)

## Indications for use



Indications for use	Patients with an aortoiliac or iliac aneurysm, an insufficient distal sealing site within the common iliac artery, and having morphology suitable for endovascular repair.	
Aneurysmal iliac	<p>Nonaneurysmal external iliac artery fixation segment distal to the aneurysm with:</p> <ul style="list-style-type: none"> <li>• Length <math>\geq 20</math> mm</li> <li>• Diameter measured outer wall to outer wall of 8-11 mm</li> </ul> <p>Nonaneurysmal internal iliac artery segment distal to the aneurysm with:</p> <ul style="list-style-type: none"> <li>• Length <math>\geq 10</math> mm (20-30 mm preferred)</li> <li>• Diameter acceptable for proper sealing</li> </ul>	
Access	Adequate femoral/iliac access compatible with the required introduction systems	
Introducer diameters	ID 20 Fr (6.7 mm) OD 7.7 mm	
Contraindications	There are no known contraindications for these devices	


# Iliac bifurcation grafts

Order Number	Reference Part Number	Distal Body Diameter mm	Common Iliac Segment Length mm	External Iliac Segment Length mm	Introducer Sheath ID/OD Fr (mm)/mm
G38612	ZBIS-10-45-41	10	45	41	20 (6.7)/7.7
G38613	ZBIS-10-45-58	10	45	58	20 (6.7)/7.7
G38616	ZBIS-12-45-41	12	45	41	20 (6.7)/7.7
G38617	ZBIS-12-45-58	12	45	58	20 (6.7)/7.7
G38614	ZBIS-10-61-41	10	61	41	20 (6.7)/7.7
G38615	ZBIS-10-61-58	10	61	58	20 (6.7)/7.7
G38618	ZBIS-12-61-41	12	61	41	20 (6.7)/7.7
G38344	ZBIS-12-61-58	12	61	58	20 (6.7)/7.7


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Introduction system for iliac bifurcation grafts

20 Fr (6.7 mm) ID/7.7 mm OD



# Iliac bifurcation grafts

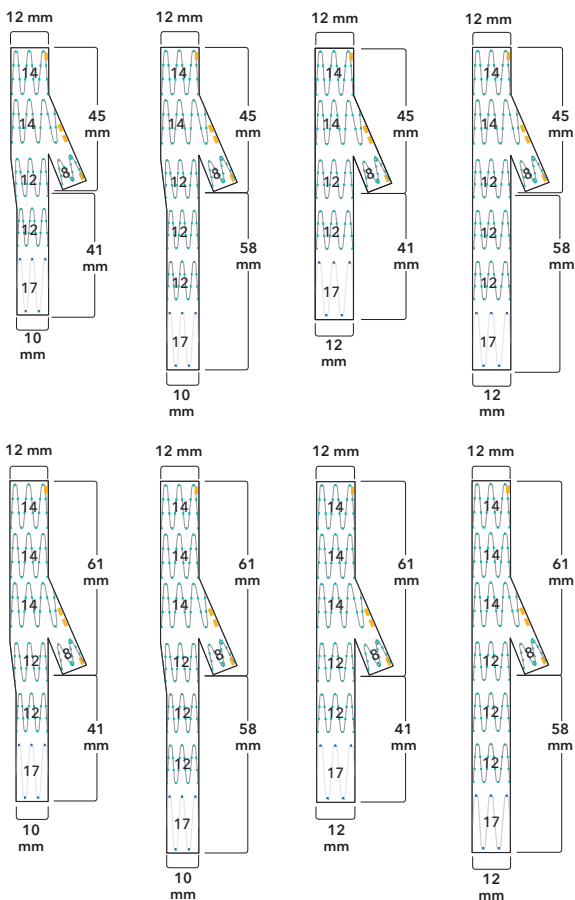

ZBIS-XX-YY-ZZ

ZBIS-(distal diameter)-(common iliac segment length)-(external iliac segment length)

Refer to [www.cookmedical.com/zenithbranch](http://www.cookmedical.com/zenithbranch) for more information.

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths.

**Note:** Zenith® Branch is compatible with 16 mm Zenith Spiral-Z® legs and Zenith Alpha™ Spiral-Z® legs.

## Deployment overview\*

### 1 PLACE THE ILIAC BRANCH

Insert the device's introduction system over the wire guide and into the iliac artery until the tip of the sheath is just above the aortic bifurcation. The distal gold marker must be at least 10 mm above the origin of the internal iliac artery.

### 2 POSITION THE BRANCH DEVICE

Position the device and withdraw the sheath until the 260 cm long stainless steel through-and-through wire guide is exposed. Advance this wire guide into the snare.

Pull the snared wire through, and place the 12 Fr Flexor® Introducer Sheath over the wire guide until the dilator tip meets the indwelling catheter tip.

Clamp the through-and-through wire guide at both ends to prevent wire guide displacement.

### 3 DEPLOY THE BRANCH DEVICE

Deploy the branch device until the distal end of the side branch is exposed.

### 4 PLACE THE UP-AND-OVER SHEATH

Advance the guiding sheath and the through-and-through wire guide together until the dilator tip stops.

### 5 POSITION THE GUIDING SHEATH

Continue to advance the sheath over the secured wire guide and into the proximal opening of the device and out through the side branch.

### 6 PUNCTURE THE HEMOSTATIC VALVE

Remove the inner dilator. Use an 18 gage needle to make an off-center puncture in the valve of the guiding sheath. Advance the access wire and the catheter through the sheath in order to access the internal iliac artery.

## Deployment overview\* (continued)

### 7 POSITION THE COVERED CONNECTING STENT

Replace the hydrophilic wire guide with a 260 cm long exchange wire guide. Advance the covered connecting stent into position. Use the distal gold aiming marker to ensure optimal overlap between the covered connecting stent and the side-branch segment. Remove the indwelling catheter and through-and-through wire guide together.

**Note:** A 7 Fr or 8 Fr Ansel sheath can be used coaxially through the 12 Fr sheath in order to introduce the covered connecting stent.

### 8 DEPLOY THE DISTAL ILIAC SEGMENT

Withdraw the device's sheath until the external iliac segment is deployed.

### 9 REMOVE THE PROXIMAL TRIGGER WIRE

Remove the proximal trigger wire in order to secure the proximal stent.

### 10 DEPLOYING THE COVERED CONNECTING STENT

Withdraw the guiding sheath until it is outside of the covered stent. Using an inflation device, deploy the covered stent


### 11 REMOVE THE DISTAL TRIGGER WIRE

Remove the distal trigger wire.

### 12 REMOVE THE INTRODUCTION SYSTEM

Withdraw the guiding sheath, balloon, and exchange wire guide. Remove the dilator from the branch device's sheath, and prepare to place the Zenith AAA graft and leg.

*\*This deployment overview is an outline highlighting the deployment process for the Zenith Branch Iliac Endovascular Graft. The Instructions for Use booklet should be consulted for a more thorough examination of the deployment protocol, indications, contraindications, warnings, and precautions.*




Insist on precise placement and unrivalled migration resistance.

# Zenith Flex<sup>®</sup>

AAA ENDOVASCULAR GRAFT

[back](#)

## Indications for use



<b>Indications for use</b>	Patients with abdominal aortic or aortoiliac aneurysms having morphology suitable for endovascular repair		
<b>Length</b>	≥ 15 mm nonaneurysmal infrarenal neck		
<b>Aortic fixation site diameter</b>	18-32 mm (measured outer wall to outer wall)		
<b>Angulation/curvature</b>	<ul style="list-style-type: none"> <li>• Angle &lt; 60 degrees relative to the long axis of the aneurysm</li> <li>• Angle &lt; 45 degrees relative to the axis of the suprarenal aorta</li> </ul>		
<b>Ipsilateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 7.5-20 mm in diameter (measured outer wall to outer wall)		
<b>Contralateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 7.5-20 mm in diameter (measured outer wall to outer wall)		
<b>Access</b>	Adequate femoral/iliac access compatible with the required introduction systems		
<b>Introducer diameters</b>	22-26 mm grafts: ID 18 Fr (6.0 mm) OD 7.1 mm	28-32 mm grafts: ID 20 Fr (6.7 mm) OD 7.7 mm	36 mm grafts: ID 22 Fr (7.3 mm) OD 8.5 mm
<b>Contraindications</b>	<ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to stainless steel, polyester, solder (tin, silver), polypropylene, or gold</li> <li>• Patients with a systemic infection who may be at increased risk of endovascular graft infection</li> </ul>		



# Bifurcated main body grafts

Order Number	Reference Part Number	Aortic Vessel OD mm	Main Body Diameter mm	Main Body Contralateral Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>					
G48402	TFFB-22-82-ZT	18-19	22	82	18 (6.0)/7.1
G48403	TFFB-22-96-ZT	18-19	22	96	18 (6.0)/7.1
G48404	TFFB-22-111-ZT	18-19	22	111	18 (6.0)/7.1
G48405	TFFB-22-125-ZT	18-19	22	125	18 (6.0)/7.1
G48406	TFFB-22-140-ZT	18-19	22	140	18 (6.0)/7.1
<b>24 mm Diameter</b>					
G48407	TFFB-24-82-ZT	20-21	24	82	18 (6.0)/7.1
G48408	TFFB-24-96-ZT	20-21	24	96	18 (6.0)/7.1
G48409	TFFB-24-111-ZT	20-21	24	111	18 (6.0)/7.1
G48410	TFFB-24-125-ZT	20-21	24	125	18 (6.0)/7.1
G48411	TFFB-24-140-ZT	20-21	24	140	18 (6.0)/7.1
<b>26 mm Diameter</b>					
G48412	TFFB-26-82-ZT	22	26	82	18 (6.0)/7.1
G48413	TFFB-26-96-ZT	22	26	96	18 (6.0)/7.1
G48414	TFFB-26-111-ZT	22	26	111	18 (6.0)/7.1
G48415	TFFB-26-125-ZT	22	26	125	18 (6.0)/7.1
G48416	TFFB-26-140-ZT	22	26	140	18 (6.0)/7.1
<b>28 mm Diameter</b>					
G48417	TFFB-28-82-ZT	23-24	28	82	20 (6.7)/7.7
G48418	TFFB-28-96-ZT	23-24	28	96	20 (6.7)/7.7
G48419	TFFB-28-111-ZT	23-24	28	111	20 (6.7)/7.7
G48420	TFFB-28-125-ZT	23-24	28	125	20 (6.7)/7.7
G48421	TFFB-28-140-ZT	23-24	28	140	20 (6.7)/7.7
<b>30 mm Diameter</b>					
G48422	TFFB-30-82-ZT	25-26	30	82	20 (6.7)/7.7
G48423	TFFB-30-96-ZT	25-26	30	96	20 (6.7)/7.7
G48424	TFFB-30-111-ZT	25-26	30	111	20 (6.7)/7.7
G48425	TFFB-30-125-ZT	25-26	30	125	20 (6.7)/7.7
G48426	TFFB-30-140-ZT	25-26	30	140	20 (6.7)/7.7

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Bifurcated main body grafts (continued)

Order Number	Reference Part Number	Aortic Vessel OD mm	Main Body Diameter mm	Main Body Contralateral Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>32 mm Diameter</b>					
G48427	TFFB-32-82-ZT	27-28	32	82	20 (6.7)/7.7
G48428	TFFB-32-96-ZT	27-28	32	96	20 (6.7)/7.7
G48429	TFFB-32-111-ZT	27-28	32	111	20 (6.7)/7.7
G48430	TFFB-32-125-ZT	27-28	32	125	20 (6.7)/7.7
G48431	TFFB-32-140-ZT	27-28	32	140	20 (6.7)/7.7
<b>36 mm Diameter</b>					
G48432	TFFB-36-95-ZT	29-32	36	95	22 (7.3)/8.5
G48433	TFFB-36-113-ZT	29-32	36	113	22 (7.3)/8.5
G48434	TFFB-36-131-ZT	29-32	36	131	22 (7.3)/8.5
G48435	TFFB-36-149-ZT	29-32	36	149	22 (7.3)/8.5


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### Z-Trak® Introduction System for main body grafts


22-26 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

28-32 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



## Bifurcated main body grafts



**Note:** Ipsilateral and contralateral limb diameters on all 22 mm diameter main body grafts are 11 mm.


TFFB-XX-YYY-ZT

TFFB-(main body diameter)-(main body contralateral length)-ZT

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

**Note:** Zenith Flex® is compatible with Zenith Spiral-Z® legs.

## Bifurcated main body grafts (continued)

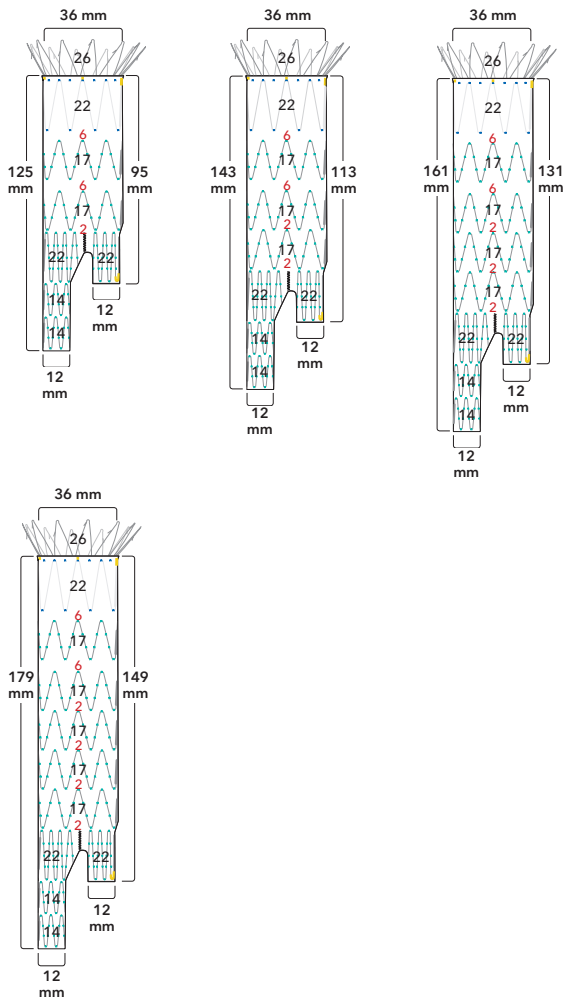

# Ancillary components

Order Number	Reference Part Number	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>Main Body Extensions</b>					
G32179	ESBE-22-39	18-19	22	39	18 (6.0)/7.1
G32180	ESBE-24-39	20-21	24	39	18 (6.0)/7.1
G32181	ESBE-26-39	22-23	26	39	18 (6.0)/7.1
G32182	ESBE-28-39	24-25	28	39	20 (6.7)/7.7
G32183	ESBE-30-39	26-27	30	39	20 (6.7)/7.7
G32184	ESBE-32-39	28	32	39	20 (6.7)/7.7
G43360	ESBE-36-50	29-32	36	50	20 (6.7)/7.7
G42783	ESBE-22-58	18-19	22	58	18 (6.0)/7.1
G42784	ESBE-24-58	20-21	24	58	18 (6.0)/7.1
G42785	ESBE-26-58	22-23	26	58	18 (6.0)/7.1
G42786	ESBE-28-58	24-25	28	58	20 (6.7)/7.7
G42787	ESBE-30-58	26-27	30	58	20 (6.7)/7.7
G42788	ESBE-32-58	28	32	58	20 (6.7)/7.7
G43361	ESBE-36-73	29-32	36	73	20 (6.7)/7.7

Order Number	Reference Part Number	Main Body Diameter mm	Proximal Diameter mm	Distal Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>Converters</b>						
G12496	ESC-24-12-80	22, 24	24	12	80	18 (6.0)/7.1
G12483	ESC-28-12-80	26, 28	28	12	80	20 (6.7)/7.7
G12484	ESC-32-12-80	30, 32	32	12	80	20 (6.7)/7.7
G43355	ESC-36-12-82	36	36	12	82	20 (6.7)/7.7


Order Number	Reference Part Number	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>Iliac Plugs</b>				
G55343	ZIP-14-ZT	14	30	14 (4.7)/5.4
G55344	ZIP-16-ZT	16	30	14 (4.7)/5.4
G55346	ZIP-20-ZT	20	30	16 (5.3)/6.0
G55348	ZIP-24-ZT	24	30	16 (5.3)/6.0

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.




# Ancillary components

## Main body extensions

22, 24, 26, 28, 30, 32 mm




22, 24, 26, 28, 30, 32 mm



## Introduction System for main body extensions

22-26 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

28-36 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD



## Main body extensions

ESBE-XX-YY


ESBE-(diameter)-(length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths.


## Ancillary components (continued)

### Converters

24, 28, 32 mm




36 mm



### Iliac plugs


14, 16, 20, 24 mm



### Introduction System for converters

24 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD


28-36 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD



### Z-Trak® Introduction System for iliac plugs

14-16 mm grafts: 14 Fr (4.7 mm) ID/5.4 mm OD

20-24 mm grafts: 16 Fr (5.3 mm) ID/6.0 mm OD



### Converters

ESC-XX-YY-ZZ

ESC-(proximal diameter)-(distal diameter)-  
(length)

### Iliac plugs

ZIP-XX-ZT

ZIP-(diameter)-ZT

# Deployment overview\*

## 1a MAIN BODY PLACEMENT

**Note:** Before insertion, position the main body introduction system on the patient's abdomen under fluoroscopy to determine the orientation of the contralateral limb radiopaque marker.

Insert the main body introduction system over the wire into the femoral artery. Advance the introduction system until the four gold radiopaque markers (which are positioned 2 mm from the most proximal segment of the graft material) are just inferior to the most inferior renal orifice.

- 1b Deploy the first two covered stents by withdrawing the sheath while monitoring the device location. Check the position of the contralateral limb radiopaque marker and the location of renal arteries.

**Note:** A marker formation of √ indicates an anterior position of the short contralateral limb.

Proceed with deployment until the contralateral limb is fully deployed. Stop withdrawing the sheath.

## 2 CONTRALATERAL ILIAC WIRE GUIDE PLACEMENT

Manipulate the catheter and wire guide through the open end of the contralateral limb into the body of the endovascular graft. A-P and oblique fluoroscopic views aid in verification of device cannulation. Advance the angiographic catheter over the wire into the body of the endovascular graft. Perform angiography to confirm position, then advance the wire guide until it curves inside the body of the endovascular graft.

## 3 MAIN BODY PROXIMAL (TOP) DEPLOYMENT

Remove the safety lock from the top stent trigger-wire release mechanism. Withdraw and remove the trigger-wire release mechanism. Loosen the pin vise and deploy the suprarenal stent by advancing the top cap inner cannula 1 to 2 mm at a time until the top stent is fully deployed. Advance the top cap inner cannula an additional 1 to 2 cm and retighten the pin vise. Advance the contralateral wire guide into the thoracic aorta.

**Note:** Once the barbed suprarenal stent has been deployed, further attempts to reposition the graft are not recommended.

## 4 CONTRALATERAL ILIAC LEG PLACEMENT AND DEPLOYMENT

Introduce the contralateral iliac leg introduction system into the artery. Advance slowly until the iliac leg graft overlaps at least one full iliac leg stent inside the contralateral limb of the main body. Reposition the iliac leg graft if necessary to ensure both internal iliac patency and a minimum of one full iliac leg stent overlap (maximum 30 mm) within the main body endovascular graft. To deploy, hold the iliac leg graft in position with the grey positioner while withdrawing the sheath. Stop withdrawing the sheath as soon as the distal end of the iliac leg graft is released. Verify the iliac leg graft position, loosen the pin vise, and retract the inner cannula to dock the tapered dilator to the grey positioner. Tighten the pin vise and withdraw the grey positioner with the secured inner cannula.

## 5 MAIN BODY DISTAL (BOTTOM) DEPLOYMENT

Fully deploy the ipsilateral limb of the main body by withdrawing the sheath until the most distal stent has expanded. Stop withdrawing the sheath. Remove the safety lock from the ipsilateral limb trigger-wire release mechanism. Withdraw and remove the trigger-wire release mechanism.



## Deployment overview\* (continued)

### 6 DOCKING OF THE TOP CAP

Loosen the pin vise and advance the grey positioner over the inner cannula until it docks with the top cap. Retighten the pin vise and withdraw the entire top cap and grey positioner through the endovascular graft and through the sheath by pulling on the inner cannula.

**Note:** Maintain the position of the sheath and wire guide.

Close the Captor® Hemostatic Valve on the Flexor® Introducer Sheath.

### 7 IPSILATERAL ILIAC LEG PLACEMENT AND DEPLOYMENT

Use the main body graft wire and sheath assembly to introduce the ipsilateral iliac leg graft. Advance the dilator and sheath assembly into the main body sheath. Advance slowly until the ipsilateral iliac leg graft overlaps a minimum of one full iliac leg stent inside the ipsilateral limb of the main body. Reposition the iliac leg graft, if necessary, to ensure internal iliac patency. To deploy, stabilise the iliac leg graft with the grey positioner while withdrawing the iliac leg sheath. Verify the iliac leg graft position, loosen the pin vise, and retract the inner cannula to dock the tapered dilator to the grey positioner. Tighten the pin vise and withdraw the grey positioner with the secured inner cannula. Close the Captor Hemostatic Valve on the Flexor Introducer Sheath.

### 8 MOLDING BALLOON INSERTION

Advance the molding balloon over the wire guide and through the hemostatic valve of the main body introduction system to the level of the renal arteries. Expand the molding balloon with diluted contrast media in the area of the most proximal covered stent and the infrarenal neck, starting proximally and working in the distal direction.

**Caution:** Confirm complete balloon deflation prior to repositioning.

**Caution:** Captor Hemostatic Valve must be open prior to repositioning of molding balloon.

Withdraw the molding balloon to both the ipsilateral limb overlap and the ipsilateral distal fixation site and expand. Deflate and remove the molding balloon. Transfer the molding balloon onto the contralateral wire guide and into the contralateral iliac leg introduction system. Advance the molding balloon to the contralateral limb overlap and expand. Withdraw the molding balloon to the contralateral iliac leg/ vessel distal fixation and expand.

**Caution:** Do not inflate the balloon in the iliac vessel outside of graft.

Deflate and remove the molding balloon and replace it with an angiographic catheter to perform completion angiography.

*\*This deployment overview is an outline highlighting the deployment process for the Zenith Flex AAA Endovascular Graft. The Instructions for Use booklet should be consulted for a more thorough examination of the deployment protocol, indications, contraindications, warnings, and precautions.*






Prioritise patency and  
system trackability.

# Zenith<sup>®</sup> Spiral-Z<sup>®</sup>

AAA ILIAC LEG GRAFT

[back](#)

## Indications for use



<b>Indications for use</b>	For use with the Zenith® AAA Endovascular Graft family of products, during either a primary or a secondary procedure in patients who have adequate iliac/femoral access compatible with the required introduction systems.	
<b>Ipsilateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 7.5-20 mm in diameter (measured outer wall to outer wall)	
<b>Contralateral iliac fixation site</b>	Distal fixation site > 10 mm in length and 7.5-20 mm in diameter (measured outer wall to outer wall)	
<b>Access</b>	Adequate femoral/iliac access compatible with the required introduction systems	
<b>Introducer diameters</b>	9-16 mm grafts: ID 14 Fr (4.7 mm) OD 5.4 mm	20-24 mm grafts: ID 16 Fr (5.3 mm) OD 6.0 mm
<b>Contraindications</b>	<ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to stainless steel, nitinol, PTFE, polyester, solder (tin, silver), polypropylene, or gold</li> <li>• Patients with a systemic or local infection who may be at increased risk of endovascular graft infection</li> </ul>	

# Contralateral/ipsilateral iliac leg grafts

Order Number	Reference Part Number	Iliac Leg Distal Diameter mm	Iliac Leg Working Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>9 mm Diameter</b>				
G55218	ZSLE-9-39-ZT	9	39	14 (4.7)/5.4
G55219	ZSLE-9-56-ZT	9	56	14 (4.7)/5.4
G55220	ZSLE-9-74-ZT	9	74	14 (4.7)/5.4
G55221	ZSLE-9-90-ZT	9	90	14 (4.7)/5.4
G55222	ZSLE-9-107-ZT	9	107	14 (4.7)/5.4
G55223	ZSLE-9-122-ZT	9	122	14 (4.7)/5.4
<b>11 mm Diameter</b>				
G55224	ZSLE-11-39-ZT	11	39	14 (4.7)/5.4
G55225	ZSLE-11-56-ZT	11	56	14 (4.7)/5.4
G55226	ZSLE-11-74-ZT	11	74	14 (4.7)/5.4
G55227	ZSLE-11-90-ZT	11	90	14 (4.7)/5.4
G55228	ZSLE-11-107-ZT	11	107	14 (4.7)/5.4
G55229	ZSLE-11-122-ZT	11	122	14 (4.7)/5.4
<b>13 mm Diameter</b>				
G55230	ZSLE-13-39-ZT	13	39	14 (4.7)/5.4
G55231	ZSLE-13-56-ZT	13	56	14 (4.7)/5.4
G55232	ZSLE-13-74-ZT	13	74	14 (4.7)/5.4
G55233	ZSLE-13-90-ZT	13	90	14 (4.7)/5.4
G55234	ZSLE-13-107-ZT	13	107	14 (4.7)/5.4
G55235	ZSLE-13-122-ZT	13	122	14 (4.7)/5.4
<b>16 mm Diameter</b>				
G55236	ZSLE-16-39-ZT	16	39	14 (4.7)/5.4
G55237	ZSLE-16-56-ZT	16	56	14 (4.7)/5.4
G55238	ZSLE-16-74-ZT	16	74	14 (4.7)/5.4
G55239	ZSLE-16-90-ZT	16	90	14 (4.7)/5.4
<b>20 mm Diameter</b>				
G55240	ZSLE-20-39-ZT	20	39	16 (5.3)/6.0
G55241	ZSLE-20-56-ZT	20	56	16 (5.3)/6.0
G55242	ZSLE-20-74-ZT	20	74	16 (5.3)/6.0
G55243	ZSLE-20-90-ZT	20	90	16 (5.3)/6.0

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Contralateral/ipsilateral iliac leg grafts (continued)


Order Number	Reference Part Number	Iliac Leg Distal Diameter mm	Iliac Leg Working Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>24 mm Diameter</b>				
G55244	ZSLE-24-39-ZT	24	39	16 (5.3)/6.0
G55245	ZSLE-24-56-ZT	24	56	16 (5.3)/6.0
G55246	ZSLE-24-74-ZT	24	74	16 (5.3)/6.0
G55247	ZSLE-24-90-ZT	24	90	16 (5.3)/6.0

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


### Z-Trak® Introduction System for iliac legs

9-16 mm grafts: 14 Fr (4.7 mm) ID/5.4 mm OD

20-24 mm grafts: 16 Fr (5.3 mm) ID/6.0 mm OD



## Contralateral/ipsilateral iliac leg grafts





ZSLE-XX-YY-ZT

ZSLE-(distal diameter)-(working length)-ZT



**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths.

## Contralateral/ipsilateral iliac leg grafts (continued)






## Contralateral/ipsilateral iliac leg grafts (continued)








Insist on precise placement and unrivalled migration resistance.

# Zenith Flex<sup>®</sup> AUI

AAA ENDOVASCULAR GRAFT

[back](#)

## Indications for use



<b>Indications for use</b>	Patients with abdominal aortic, ruptured abdominal aortic, aortoiliac, or iliac aneurysms having morphology suitable for endovascular repair.		
<b>Length</b>	$\geq 15$ mm nonaneurysmal infrarenal neck		
<b>Aortic fixation site diameter</b>	18-32 mm (measured outer wall to outer wall)		
<b>Angulation/curvature</b>	<ul style="list-style-type: none"> <li>• Angle <math>&lt; 60</math> degrees relative to the long axis of the aneurysm; and</li> <li>• Angle <math>&lt; 45</math> degrees relative to the axis of the suprarenal aorta.</li> </ul>		
<b>Ipsilateral iliac fixation site</b>	Distal fixation site 7.5-20 mm in diameter (outer wall to outer wall) and $> 10$ mm in length (20 mm preferred)		
<b>Contralateral iliac fixation site</b>	Iliac Plug (ZIP) available for occlusion when femoral-to-femoral crossover is required		
<b>Access</b>	Adequate femoral/iliac access compatible with the required introduction systems		
<b>Introducer diameters</b>	22, 24, 26 mm grafts: ID 18 Fr (6.0 mm) OD 7.1 mm	28-32 mm grafts: ID 20 Fr (6.7 mm) OD 7.7 mm	36 mm grafts: ID 22 Fr (7.3 mm) OD 8.5 mm
<b>Contraindications</b>	<p>The Zenith Flex AUI AAA Endovascular Graft with the Z-Trak Introduction System is contraindicated in:</p> <ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to stainless steel, polyester, solder (tin, silver), polypropylene, or gold</li> <li>• Patients with systemic infection who may be at increased risk of endovascular graft infection</li> </ul>		

## Aortouniliac (AUI) main body grafts

Order Number	Reference Part Number	Aortic Vessel OD mm	Main Body Proximal Diameter mm	Main Body Distal Diameter mm	Main Body Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>						
G53799	ZAUI-22-130-ZT	18-19	22	12	130	18 (6.0)/7.1
<b>24 mm Diameter</b>						
G53802	ZAUI-24-130-ZT	20-21	24	12	130	18 (6.0)/7.1
G53803	ZAUI-24-147-ZT	20-21	24	12	147	18 (6.0)/7.1
<b>26 mm Diameter</b>						
G53805	ZAUI-26-130-ZT	22	26	12	130	18 (6.0)/7.1
<b>28 mm Diameter</b>						
G53808	ZAUI-28-130-ZT	23-24	28	12	130	20 (6.7)/7.7
G53809	ZAUI-28-147-ZT	23-24	28	12	147	20 (6.7)/7.7
<b>30 mm Diameter</b>						
G53811	ZAUI-30-130-ZT	25-26	30	12	130	20 (6.7)/7.7
<b>32 mm Diameter</b>						
G53814	ZAUI-32-130-ZT	27-28	32	12	130	20 (6.7)/7.7
G53815	ZAUI-32-147-ZT	27-28	32	12	147	20 (6.7)/7.7
<b>36 mm Diameter</b>						
G53817	ZAUI-36-144-ZT	29-32	36	12	144	22 (7.3)/8.5
G53818	ZAUI-36-161-ZT	29-32	36	12	161	22 (7.3)/8.5


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### Z-Trak® Introduction System for main body grafts


22-26 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

28-32 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



# Aortouniiliac (AUI) main body grafts




ZAUI-XX-YYY-ZT

ZAUI-(proximal diameter)-(main body length)-ZT

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

**Note:** Zenith Flex® AUI is compatible with Zenith Spiral-Z® legs.




Restore graft-to-vessel  
fixation and seal.

# Zenith Renu<sup>®</sup>

AAA ANCILLARY GRAFT

[back](#)

## Indications for use



<b>Indications for use</b>	Secondary endovascular intervention in patients having received prior endovascular repair of infrarenal abdominal aortic or aortoiliac aneurysms in which there is inadequate proximal fixation or seal.		
<b>Length</b>	Lowest renal artery to bifurcation of previously placed graft of $> 43$ mm for the main body extension and $> 37$ mm for the converter.		
<b>Aortic fixation site diameter</b>	18-32 mm (measured outer wall to outer wall)		
<b>Angulation/curvature</b>	<ul style="list-style-type: none"> <li>• Angle <math>&lt; 60</math> degrees relative to the long axis of the aneurysm</li> <li>• Angle <math>&lt; 45</math> degrees relative to the axis of the suprarenal aorta</li> </ul>		
<b>Converter distal fixation site</b>	For the converter used without an iliac leg, distal fixation site within a graft segment of $\leq 12$ mm in diameter and $\geq 17$ mm (one Cook-Z <sup>®</sup> stent) in length, with more overlap length being preferred. For the converter used in combination with the iliac leg, distal fixation site 7.5-20 mm in diameter (measured outer wall to outer wall) and $> 10$ mm in length with 20 to 30 mm being preferred.		
<b>Main body distal fixation site</b>	Main body extension distal fixation site within a graft segment of $\leq 34$ mm diameter and at least one Cook-Z stent in length, with more overlap length being preferred.		
<b>Access</b>	Adequate femoral/iliac access compatible with the required introduction systems		
<b>Introducer diameters</b>	22-26 mm grafts: ID 18 Fr (6.0 mm) OD 7.1 mm	28-32 mm grafts: ID 20 Fr (6.7 mm) OD 7.7 mm	36 mm grafts: ID 22 Fr (7.3 mm) OD 8.5 mm
<b>Contraindications</b>	<ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to stainless steel, polyester, solder (tin, silver), polypropylene, or gold</li> <li>• Patients with a systemic infection who may be at increased risk of endovascular graft infection</li> </ul>		



# Converters

Order Number	Reference Part Number	Aortic Vessel OD* mm	Proximal/ Distal Diameter mm	Proximal/ Distal Length mm	Total Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>						
G36147	AX1-1-22-108	18-19	22/12	37/71	108	18 (6.0)/7.1
G36148	AX1-1-22-125	18-19	22/12	37/88	125	18 (6.0)/7.1
<b>24 mm Diameter</b>						
G36153	AX1-1-24-108	20-21	24/12	37/71	108	18 (6.0)/7.1
G36154	AX1-1-24-125	20-21	24/12	37/88	125	18 (6.0)/7.1
<b>26 mm Diameter</b>						
G36159	AX1-1-26-108	22	26/12	37/71	108	18 (6.0)/7.1
G36160	AX1-1-26-125	22	26/12	37/88	125	18 (6.0)/7.1
<b>28 mm Diameter</b>						
G36165	AX1-1-28-108	23-24	28/12	37/71	108	20 (6.7)/7.7
G36166	AX1-1-28-125	23-24	28/12	37/88	125	20 (6.7)/7.7
<b>30 mm Diameter</b>						
G36171	AX1-1-30-108	25-26	30/12	37/71	108	20 (6.7)/7.7
G36172	AX1-1-30-125	25-26	30/12	37/88	125	20 (6.7)/7.7
<b>32 mm Diameter</b>						
G36177	AX1-1-32-108	27-28	32/12	37/71	108	20 (6.7)/7.7
G36178	AX1-1-32-125	27-28	32/12	37/88	125	20 (6.7)/7.7
<b>36 mm Diameter</b>						
G43370	AX1-1-36-116	29-32	36/12	52/64	116	22 (7.3)/8.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


\*Maximum diameter along the proximal fixation site. Round measured aortic diameter to nearest mm. Additional considerations may affect choice of diameter.

## H&L-B One-Shot Introduction System for Renu converters


22-26 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

28-32 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



# Converters



AX1-1-XX-YYY

AX1-1-(proximal diameter)-(total length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

**Note:** Zenith Renu® is compatible with Zenith Spiral-Z® legs.

## Main body extensions

Order Number	Reference Part Number	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>					
G36128	RX1-22-43	18-19	22	43	18 (6.0)/7.1
G36129	RX1-22-62	18-19	22	62	18 (6.0)/7.1
<b>24 mm Diameter</b>					
G36131	RX1-24-43	20-21	24	43	18 (6.0)/7.1
G36132	RX1-24-62	20-21	24	62	18 (6.0)/7.1
<b>26 mm Diameter</b>					
G36134	RX1-26-43	22	26	43	18 (6.0)/7.1
G36135	RX1-26-62	22	26	62	18 (6.0)/7.1
<b>28 mm Diameter</b>					
G36137	RX1-28-43	23-24	28	43	20 (6.7)/7.7
G36138	RX1-28-62	23-24	28	62	20 (6.7)/7.7
<b>30 mm Diameter</b>					
G36140	RX1-30-43	25-26	30	43	20 (6.7)/7.7
G36141	RX1-30-62	25-26	30	62	20 (6.7)/7.7
<b>32 mm Diameter</b>					
G36143	RX1-32-43	27-28	32	43	20 (6.7)/7.7
G36144	RX1-32-62	27-28	32	62	20 (6.7)/7.7
<b>36 mm Diameter</b>					
G43362	RX1-36-54	29-32	36	54	22 (7.3)/8.5


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### H&L-B One-Shot Introduction System for Renu main body extensions


22-26 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

28-32 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD




## Main body extensions



RX1-XX-YY

RX1-(diameter)-(length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

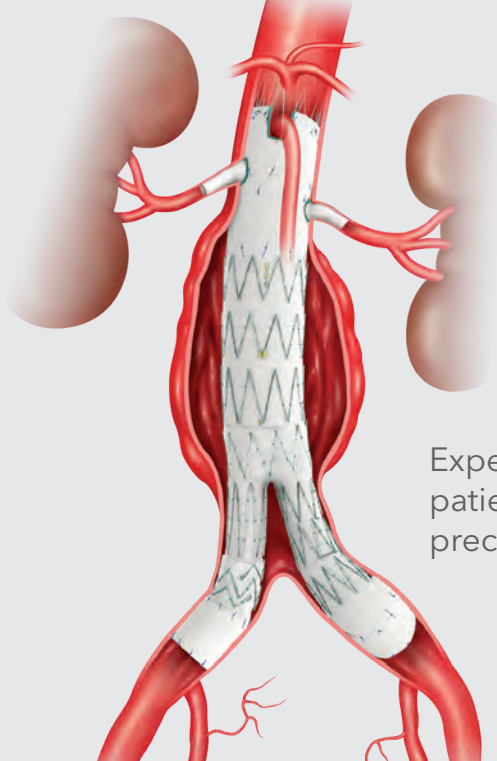


Experience  
patient-specific  
precision.

# Zenith<sup>®</sup> Fenestrated

AAA ENDOVASCULAR GRAFT

[back](#)

## Indications for use



Indications for use	Infrarenal abdominal aortic aneurysms (AAAs) in high-risk patients who are not suitable for conventional open surgical repair or who are not suitable for repair with a standard Zenith Endovascular Graft, when the aneurysmal disease extends up to the level of the renal arteries.		
Length	≥ 4 mm nonaneurysmal neck		
Aortic fixation site diameter	19-31 mm (measured outer wall to outer wall)		
Angulation/curvature	<ul style="list-style-type: none"> <li>• Angle &lt; 45 degrees relative to the long axis of the aneurysm</li> <li>• Angle &lt; 45 degrees relative to the axis of the suprarenal aorta</li> </ul>		
Ipsilateral iliac fixation site	Distal fixation site > 10 mm in length and 9-21 mm in diameter (measured outer wall to outer wall)		
Contralateral iliac fixation site	Distal fixation site > 10 mm in length and 7-21 mm in diameter (measured outer wall to outer wall)		
Access	Adequate femoral/iliac access compatible with the required introduction systems		
Introducer diameters	24-34 mm grafts: ID 20 Fr (6.7 mm) OD 7.7 mm	36 mm grafts: ID 22 Fr (7.3 mm) OD 8.5 mm	
Contraindications	There are no known contraindications for these devices.		

# Proximal body grafts

Order Number	Reference Part Number	Aortic Vessel OD mm	Proximal Body Diameter mm	Proximal Body Length mm	Introducer Sheath ID/OD Fr (mm)/7.7
<b>One Proximal Internal Stent</b>					
<b>24 mm Diameter</b>					
G38124	ZFEN-P-1-24-76	19-21	24	76	20 (6.7)/7.7
G38125	ZFEN-P-1-24-91	19-21	24	91	20 (6.7)/7.7
G38122	ZFEN-P-1-24-106	19-21	24	106	20 (6.7)/7.7
G38123	ZFEN-P-1-24-121	19-21	24	121	20 (6.7)/7.7
<b>26 mm Diameter</b>					
G38128	ZFEN-P-1-26-76	21-22	26	76	20 (6.7)/7.7
G38129	ZFEN-P-1-26-91	21-22	26	91	20 (6.7)/7.7
G38126	ZFEN-P-1-26-106	21-22	26	106	20 (6.7)/7.7
G38127	ZFEN-P-1-26-121	21-22	26	121	20 (6.7)/7.7
<b>28 mm Diameter</b>					
G38132	ZFEN-P-1-28-76	23-24	28	76	20 (6.7)/7.7
G38133	ZFEN-P-1-28-91	23-24	28	91	20 (6.7)/7.7
G38130	ZFEN-P-1-28-106	23-24	28	106	20 (6.7)/7.7
G38131	ZFEN-P-1-28-121	23-24	28	121	20 (6.7)/7.7
<b>30 mm Diameter</b>					
G38136	ZFEN-P-1-30-76	24-26	30	76	20 (6.7)/7.7
G38137	ZFEN-P-1-30-91	24-26	30	91	20 (6.7)/7.7
G38134	ZFEN-P-1-30-106	24-26	30	106	20 (6.7)/7.7
G38135	ZFEN-P-1-30-121	24-26	30	121	20 (6.7)/7.7
<b>32 mm Diameter</b>					
G38140	ZFEN-P-1-32-76	26-28	32	76	20 (6.7)/7.7
G38141	ZFEN-P-1-32-91	26-28	32	91	20 (6.7)/7.7
G38138	ZFEN-P-1-32-106	26-28	32	106	20 (6.7)/7.7
G38139	ZFEN-P-1-32-121	26-28	32	121	20 (6.7)/7.7
<b>34 mm Diameter</b>					
G38144	ZFEN-P-1-34-84	28-29	34	84	20 (6.7)/7.7
G38145	ZFEN-P-1-34-99	28-29	34	99	20 (6.7)/7.7
G38142	ZFEN-P-1-34-114	28-29	34	114	20 (6.7)/7.7
G38143	ZFEN-P-1-34-129	28-29	34	129	20 (6.7)/7.7
<b>36 mm Diameter</b>					
G38148	ZFEN-P-1-36-84	29-31	36	84	22 (7.3)/8.5
G38149	ZFEN-P-1-36-99	29-31	36	99	22 (7.3)/8.5
G38146	ZFEN-P-1-36-114	29-31	36	114	22 (7.3)/8.5
G38147	ZFEN-P-1-36-129	29-31	36	129	22 (7.3)/8.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Proximal body grafts (continued)


Order Number	Reference Part Number	Aortic Vessel OD mm	Proximal Body Diameter mm	Proximal Body Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>Two Proximal Internal Stents</b>					
<b>24 mm Diameter</b>					
G38152	ZFEN-P-2-24-94	19-21	24	94	20 (6.7)/7.7
G38150	ZFEN-P-2-24-109	19-21	24	109	20 (6.7)/7.7
G38151	ZFEN-P-2-24-124	19-21	24	124	20 (6.7)/7.7
<b>26 mm Diameter</b>					
G38155	ZFEN-P-2-26-94	21-22	26	94	20 (6.7)/7.7
G38153	ZFEN-P-2-26-109	21-22	26	109	20 (6.7)/7.7
G38154	ZFEN-P-2-26-124	21-22	26	124	20 (6.7)/7.7
<b>28 mm Diameter</b>					
G38158	ZFEN-P-2-28-94	23-24	28	94	20 (6.7)/7.7
G38156	ZFEN-P-2-28-109	23-24	28	109	20 (6.7)/7.7
G38157	ZFEN-P-2-28-124	23-24	28	124	20 (6.7)/7.7
<b>30 mm Diameter</b>					
G38161	ZFEN-P-2-30-94	24-26	30	94	20 (6.7)/7.7
G38159	ZFEN-P-2-30-109	24-26	30	109	20 (6.7)/7.7
G38160	ZFEN-P-2-30-124	24-26	30	124	20 (6.7)/7.7
<b>32 mm Diameter</b>					
G38164	ZFEN-P-2-32-94	26-28	32	94	20 (6.7)/7.7
G38162	ZFEN-P-2-32-109	26-28	32	109	20 (6.7)/7.7
G38163	ZFEN-P-2-32-124	26-28	32	124	20 (6.7)/7.7
<b>34 mm Diameter</b>					
G38165	ZFEN-P-2-34-107	28-29	34	107	20 (6.7)/7.7
G38166	ZFEN-P-2-34-122	28-29	34	122	20 (6.7)/7.7
G38167	ZFEN-P-2-34-137	28-29	34	137	20 (6.7)/7.7
<b>36 mm Diameter</b>					
G38168	ZFEN-P-2-36-107	29-31	36	107	22 (7.3)/8.5
G38169	ZFEN-P-2-36-122	29-31	36	122	22 (7.3)/8.5
G38170	ZFEN-P-2-36-137	29-31	36	137	22 (7.3)/8.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### H&L-B One-Shot® Introduction System for proximal body grafts

24-34 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD


36 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD





# Proximal body grafts

One proximal internal stent

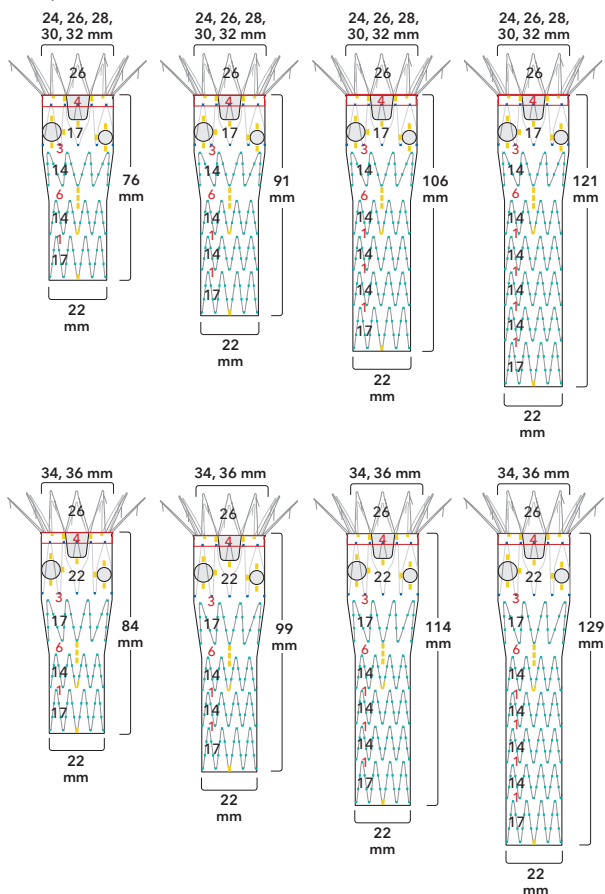

ZFEN-P-1-XX-YYY



ZFEN-P-1-(proximal body diameter)-(proximal body length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

# Proximal body grafts (continued)

## Two proximal internal stents

24, 26, 28, 30, 32 mm    24, 26, 28, 30, 32 mm    24, 26, 28, 30, 32 mm



ZFEN-P-2-XX-YYY

ZFEN-P-2-(proximal body diameter)-(proximal body length)

## Distal bifurcated body grafts

Order Number	Reference Part Number	Ipsilateral Leg Diameter mm	Distal Ipsilateral Leg Length mm	Distal Body Length mm	Introducer Sheath ID/OD Fr (mm)/mm
G38079	ZFEN-D-12-28-76	12	28	76	20 (6.7)/7.7
G38574	ZFEN-D-12-28-94	12	28	94	20 (6.7)/7.7
G38577	ZFEN-D-12-28-109	12	28	109	20 (6.7)/7.7
G38580	ZFEN-D-12-28-124	12	28	124	20 (6.7)/7.7
G38083	ZFEN-D-12-45-76	12	45	76	20 (6.7)/7.7
G38583	ZFEN-D-12-45-94	12	45	94	20 (6.7)/7.7
G38587	ZFEN-D-12-45-109	12	45	109	20 (6.7)/7.7
G38591	ZFEN-D-12-45-124	12	45	124	20 (6.7)/7.7
G38087	ZFEN-D-12-62-76	12	62	76	20 (6.7)/7.7
G38595	ZFEN-D-12-62-94	12	62	94	20 (6.7)/7.7
G38599	ZFEN-D-12-62-109	12	62	109	20 (6.7)/7.7
G38603	ZFEN-D-12-62-124	12	62	124	20 (6.7)/7.7
G38091	ZFEN-D-16-28-76	16	28	76	20 (6.7)/7.7
G38575	ZFEN-D-16-28-94	16	28	94	20 (6.7)/7.7
G38578	ZFEN-D-16-28-109	16	28	109	20 (6.7)/7.7
G38581	ZFEN-D-16-28-124	16	28	124	20 (6.7)/7.7
G38095	ZFEN-D-16-45-76	16	45	76	20 (6.7)/7.7
G38584	ZFEN-D-16-45-94	16	45	94	20 (6.7)/7.7
G38588	ZFEN-D-16-45-109	16	45	109	20 (6.7)/7.7
G38592	ZFEN-D-16-45-124	16	45	124	20 (6.7)/7.7
G38099	ZFEN-D-16-62-76	16	62	76	20 (6.7)/7.7
G38596	ZFEN-D-16-62-94	16	62	94	20 (6.7)/7.7
G38600	ZFEN-D-16-62-109	16	62	109	20 (6.7)/7.7
G38604	ZFEN-D-16-62-124	16	62	124	20 (6.7)/7.7
G38103	ZFEN-D-20-28-76	20	28	76	20 (6.7)/7.7
G38576	ZFEN-D-20-28-94	20	28	94	20 (6.7)/7.7
G38579	ZFEN-D-20-28-109	20	28	109	20 (6.7)/7.7
G38582	ZFEN-D-20-28-124	20	28	124	20 (6.7)/7.7
G38107	ZFEN-D-20-45-76	20	45	76	20 (6.7)/7.7
G38585	ZFEN-D-20-45-94	20	45	94	20 (6.7)/7.7
G38589	ZFEN-D-20-45-109	20	45	109	20 (6.7)/7.7
G38593	ZFEN-D-20-45-124	20	45	124	20 (6.7)/7.7

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


## Distal bifurcated body grafts (continued)

Order Number	Reference Part Number	Ipsilateral Leg Diameter mm	Distal Ipsilateral Leg Length mm	Distal Body Length mm	Introducer Sheath ID/OD Fr (mm)/mm
G38111	ZFEN-D-20-62-76	20	62	76	20 (6.7)/7.7
G38597	ZFEN-D-20-62-94	20	62	94	20 (6.7)/7.7
G38601	ZFEN-D-20-62-109	20	62	109	20 (6.7)/7.7
G38605	ZFEN-D-20-62-124	20	62	124	20 (6.7)/7.7
G38115	ZFEN-D-24-45-76	24	45	76	20 (6.7)/7.7
G38586	ZFEN-D-24-45-94	24	45	94	20 (6.7)/7.7
G38590	ZFEN-D-24-45-109	24	45	109	20 (6.7)/7.7
G38594	ZFEN-D-24-45-124	24	45	124	20 (6.7)/7.7
G38119	ZFEN-D-24-62-76	24	62	76	20 (6.7)/7.7
G38598	ZFEN-D-24-62-94	24	62	94	20 (6.7)/7.7
G38602	ZFEN-D-24-62-109	24	62	109	20 (6.7)/7.7
G38606	ZFEN-D-24-62-124	24	62	124	20 (6.7)/7.7


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### H&L-B One-Shot Introduction System for distal bifurcated body grafts

20 Fr (6.7 mm) ID/7.7 mm OD



## Distal bifurcated body grafts

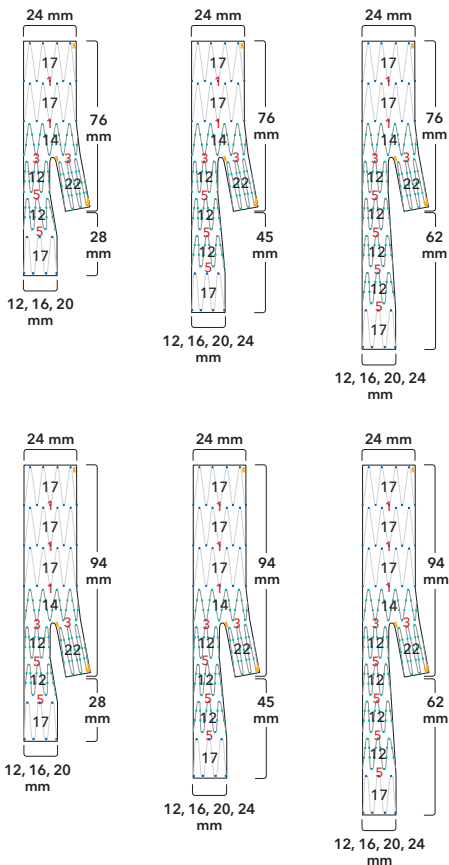







ZFEN-D-XX-YY-ZZZ

ZFEN-D-(ipsilateral leg diameter)-(distal ipsilateral leg length)-(distal body length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

**Note:** Zenith® Fenestrated is compatible with Zenith Spiral-Z® legs.

# Distal bifurcated body grafts (continued)






Designed to help  
you meet the  
challenges of  
aortic disease.

# Zenith Alpha™

THORACIC ENDOVASCULAR GRAFT

[back](#)

## Indications for use

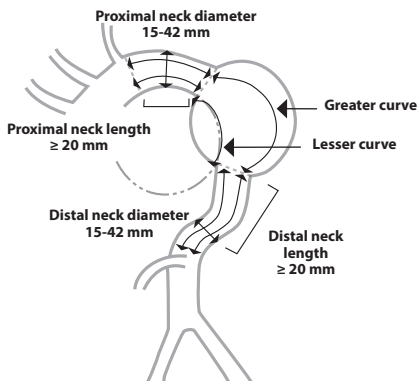

Indications for use	<p>The Zenith Alpha™ Thoracic Endovascular Graft is indicated for the endovascular treatment of patients with aneurysms/ulcers of the descending thoracic aorta having vascular morphology suitable for endovascular repair including:</p> <ul style="list-style-type: none"> <li>• Iliac/femoral anatomy that is suitable for access with the required introduction systems,</li> <li>• Nonaneurysmal aortic segments (fixation sites) proximal and distal to the aneurysm or ulcer:               <ul style="list-style-type: none"> <li>- with a length of at least 20 mm, and</li> <li>- with a diameter measured outer wall to outer wall of no greater than 42 mm and no less than 15 mm.</li> </ul> </li> </ul>		
Length	Nonaneurysmal aortic necks proximal and distal to the aneurysm with a length $\geq 20$ mm		
Aortic fixation site diameter	15-42 mm (measured outer wall to outer wall)		
Angulation/curvature	<ul style="list-style-type: none"> <li>• Radius of curvature <math>\geq 20</math> mm for aortic arch landing zones</li> <li>• An angle <math>\leq 45</math> degrees (any angle in the arch or distal aorta)</li> </ul>		
Access	Iliac/femoral anatomy that is suitable for access with the required introduction system		
Introducer diameters	18-30 mm grafts: ID 16 Fr (5.3 mm) OD 6.0 mm	32-38 mm grafts: ID 18 Fr (6.0 mm) OD 7.1 mm	40-46 mm grafts: ID 20 Fr (6.7 mm) OD 7.7 mm
Contraindications	<ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to polyester, polypropylene, nitinol, or gold.</li> <li>• Patients with a systemic infection who may be at increased risk of endovascular graft infection.</li> </ul>		



# Proximal components

Order Number	Reference Part Number	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>18 mm Diameter</b>					
G34671	ZTA-P-18-105	15-16	18	105	16 (5.3)/6.0
<b>20 mm Diameter</b>					
G34673	ZTA-P-20-105	17	20	105	16 (5.3)/6.0
<b>22 mm Diameter</b>					
G34675	ZTA-P-22-105	18-19	22	105	16 (5.3)/6.0
<b>24 mm Diameter</b>					
G34677	ZTA-P-24-105	20-21	24	105	16 (5.3)/6.0
<b>26 mm Diameter</b>					
G34679	ZTA-P-26-105	22-23	26	105	16 (5.3)/6.0
<b>28 mm Diameter</b>					
G34682	ZTA-P-28-109	24-25	28	109	16 (5.3)/6.0
G34683	ZTA-P-28-155	24-25	28	155	16 (5.3)/6.0
G34684	ZTA-P-28-201	24-25	28	201	16 (5.3)/6.0
<b>30 mm Diameter</b>					
G34685	ZTA-P-30-109	26-27	30	109	16 (5.3)/6.0
G34687	ZTA-P-30-155	26-27	30	155	16 (5.3)/6.0
G34688	ZTA-P-30-201	26-27	30	201	16 (5.3)/6.0
<b>32 mm Diameter</b>					
G34689	ZTA-P-32-109	28-29	32	109	18 (6.0)/7.1
G34691	ZTA-P-32-155	28-29	32	155	18 (6.0)/7.1
G34692	ZTA-P-32-201	28-29	32	201	18 (6.0)/7.1
<b>34 mm Diameter</b>					
G34694	ZTA-P-34-113	30	34	113	18 (6.0)/7.1
G34696	ZTA-P-34-161	30	34	161	18 (6.0)/7.1
G34697	ZTA-P-34-209	30	34	209	18 (6.0)/7.1
<b>36 mm Diameter</b>					
G34698	ZTA-P-36-113	31-32	36	113	18 (6.0)/7.1
G34700	ZTA-P-36-161	31-32	36	161	18 (6.0)/7.1
G34701	ZTA-P-36-209	31-32	36	209	18 (6.0)/7.1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Proximal components (continued)

Order Number	Reference Part Number	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>38 mm Diameter</b>					
G34702	ZTA-P-38-117	33-34	38	117	18 (6.0)/7.1
G34704	ZTA-P-38-167	33-34	38	167	18 (6.0)/7.1
G34705	ZTA-P-38-217	33-34	38	217	18 (6.0)/7.1
<b>40 mm Diameter</b>					
G34706	ZTA-P-40-117	35-36	40	117	20 (6.7)/7.7
G34708	ZTA-P-40-167	35-36	40	167	20 (6.7)/7.7
G34709	ZTA-P-40-217	35-36	40	217	20 (6.7)/7.7
<b>42 mm Diameter</b>					
G34710	ZTA-P-42-121	37-38	42	121	20 (6.7)/7.7
G34713	ZTA-P-42-173	37-38	42	173	20 (6.7)/7.7
G34714	ZTA-P-42-225	37-38	42	225	20 (6.7)/7.7
<b>44 mm Diameter</b>					
G34715	ZTA-P-44-125	39	44	125	20 (6.7)/7.7
G34717	ZTA-P-44-179	39	44	179	20 (6.7)/7.7
G34718	ZTA-P-44-233	39	44	233	20 (6.7)/7.7
<b>46 mm Diameter</b>					
G34719	ZTA-P-46-125	40-42	46	125	20 (6.7)/7.7
G34721	ZTA-P-46-179	40-42	46	179	20 (6.7)/7.7
G34722	ZTA-P-46-233	40-42	46	233	20 (6.7)/7.7


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### Introduction system for proximal components


18-30 mm grafts: 16 Fr (5.3 mm) ID/6.0 mm OD

32-38 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

40-46 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD



# Proximal components

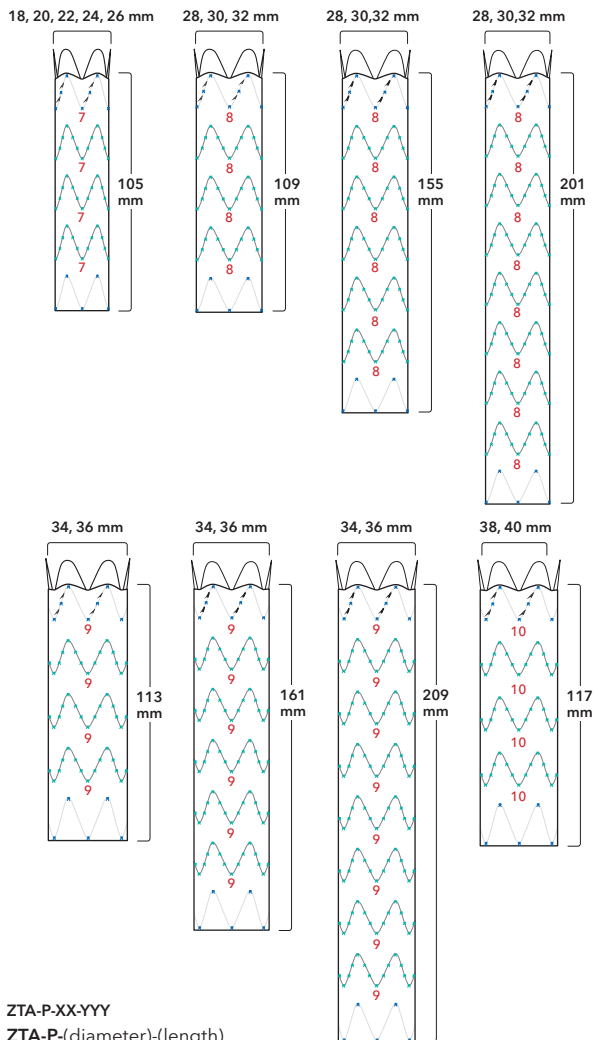


ZTA-P-XX-YYY

ZTA-P-(diameter)-(length)

**Note:** All measurements are in millimetres. Red numbers indicate gap lengths. Gap lengths are approximate.

# Proximal components (continued)

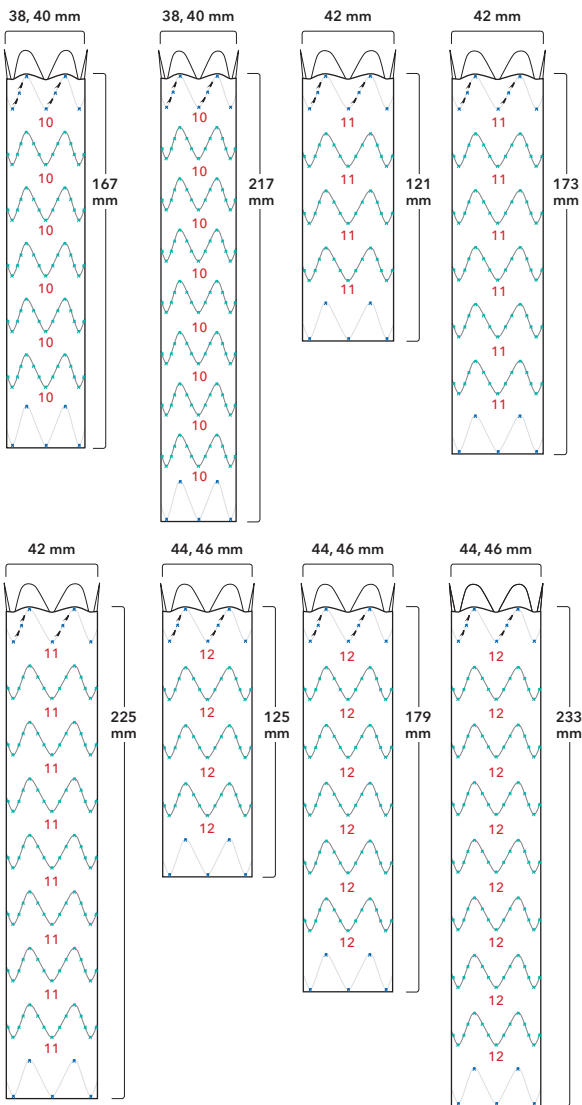

## Proximal 4 mm tapered components


Order Number	Reference Part Number	Aortic Vessel OD mm	Proximal Diameter mm	Distal Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>32 mm Diameter</b>						
G34638	ZTA-PT-32-28-178	28-29	32	28	178	18 (6.0)/7.1
G34639	ZTA-PT-32-28-201	28-29	32	28	201	18 (6.0)/7.1
<b>34 mm Diameter</b>						
G34640	ZTA-PT-34-30-161	30	34	30	161	18 (6.0)/7.1
G34642	ZTA-PT-34-30-209	30	34	30	209	18 (6.0)/7.1
<b>36 mm Diameter</b>						
G34643	ZTA-PT-36-32-161	31-32	36	32	161	18 (6.0)/7.1
G34645	ZTA-PT-36-32-209	31-32	36	32	209	18 (6.0)/7.1
<b>38 mm Diameter</b>						
G34646	ZTA-PT-38-34-167	33-34	38	34	167	18 (6.0)/7.1
G34648	ZTA-PT-38-34-217	33-34	38	34	217	18 (6.0)/7.1
<b>40 mm Diameter</b>						
G34650	ZTA-PT-40-36-167	35-36	40	36	167	20 (6.7)/7.7
G34652	ZTA-PT-40-36-217	35-36	40	36	217	20 (6.7)/7.7
<b>42 mm Diameter</b>						
G34653	ZTA-PT-42-38-173	37-38	42	38	173	20 (6.7)/7.7
G34655	ZTA-PT-42-38-225	37-38	42	38	225	20 (6.7)/7.7
<b>44 mm Diameter</b>						
G34656	ZTA-PT-44-40-179	39	44	40	179	20 (6.7)/7.7
G34657	ZTA-PT-44-40-233	39	44	40	233	20 (6.7)/7.7
<b>46 mm Diameter</b>						
G34659	ZTA-PT-46-42-179	40-42	46	42	179	20 (6.7)/7.7
G34661	ZTA-PT-46-42-233	40-42	46	42	233	20 (6.7)/7.7

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


### Introduction system for proximal 4 mm tapered components

32-38 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

40-46 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD



## Proximal 4 mm tapered components




ZTA-PT-XX-YY-ZZZ

ZTA-PT-(proximal diameter)-(distal diameter)-(length)


**Note:** All measurements are in millimetres. Red numbers indicate gap lengths.

Gap lengths are approximate.

# Proximal 4 mm tapered components (continued)




## Proximal 4 mm tapered components (continued)





## Proximal 4 mm tapered components (continued)



# Distal components

Order Number	Reference Part Number	Aortic Vessel OD mm	Distal Component Diameter mm	Distal Component Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>28 mm Diameter</b>					
G34602	ZTA-D-28-160	24-25	28	160	16 (5.3)/6.0
<b>30 mm Diameter</b>					
G34610	ZTA-D-30-160	26-27	30	160	16 (5.3)/6.0
<b>32 mm Diameter</b>					
G34619	ZTA-D-32-160	28-29	32	160	18 (6.0)/7.1
<b>34 mm Diameter</b>					
G34647	ZTA-D-34-190	30	34	190	18 (6.0)/7.1
<b>36 mm Diameter</b>					
G34651	ZTA-D-36-190	31-32	36	190	18 (6.0)/7.1
<b>38 mm Diameter</b>					
G34658	ZTA-D-38-197	33-34	38	197	18 (6.0)/7.1
<b>40 mm Diameter</b>					
G34662	ZTA-D-40-197	35-36	40	197	20 (6.7)/7.7
<b>42 mm Diameter</b>					
G34664	ZTA-D-42-204	37-38	42	204	20 (6.7)/7.7
<b>44 mm Diameter</b>					
G34667	ZTA-D-44-211	39	44	211	20 (6.7)/7.7
<b>46 mm Diameter</b>					
G34670	ZTA-D-46-211	40-41	46	211	20 (6.7)/7.7


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Introduction system for distal components


28-30 mm grafts: 16 Fr (5.3 mm) ID/6.0 mm OD

32-38 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

40-46 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD



## Distal components




ZTA-D-XX-YYY

ZTA-D-(diameter)-(distal component length)

**Note:** All measurements are in millimetres. Red numbers indicate gap lengths.

Gap lengths are approximate.

## Distal components (continued)



## Distal extensions

Order Number	Reference Part Number	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>					
G34605	ZTA-DE-22-104	18-19	22	104	16 (5.3)/6.0
<b>26 mm Diameter</b>					
G34607	ZTA-DE-26-104	22-23	26	104	16 (5.3)/6.0
<b>30 mm Diameter</b>					
G34611	ZTA-DE-30-108	26-27	30	108	16 (5.3)/6.0
<b>34 mm Diameter</b>					
G34613	ZTA-DE-34-112	30	34	112	18 (6.0)/7.1
<b>38 mm Diameter</b>					
G34616	ZTA-DE-38-91	33-34	38	91	18 (6.0)/7.1
<b>42 mm Diameter</b>					
G34618	ZTA-DE-42-94	37-38	42	94	20 (6.7)/7.7
<b>46 mm Diameter</b>					
G34622	ZTA-DE-46-97	40-42	46	97	20 (6.7)/7.7


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

### Introduction system for distal extensions

22-30 mm grafts: 16 Fr (5.3 mm) ID/6.0 mm OD


34-38 mm grafts: 18 Fr (6.0 mm) ID/7.1 mm OD

42-46 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD




## Distal extensions


22, 26 mm




30 mm




34 mm




38 mm



42 mm



46 mm



ZTA-DE-XX-YYY

ZTA-DE-(diameter)-(length)

**Note:** All measurements are in millimetres. Red numbers indicate gap lengths. Gap lengths are approximate.

# Deployment overview

## 1 POSITION THE LUNDERQUIST® EXTRA-STIFF DC WIRE GUIDE IN AORTIC ARCH

Through the pigtail flush catheter, replace the standard wire guide with an extra-stiff, .035 inch, 260 or 300 cm double-curved Lunderquist wire guide up to the level of the aortic arch and remove the pigtail.

## 2 POSITION THE PROXIMAL COMPONENT

Introduce the introduction system for the proximal component over the extra-stiff double-curved Lunderquist wire guide and advance until you reach the desired graft position.

**Caution:** To avoid twisting the graft, never rotate the introduction system during the procedure. Allow the device to conform naturally. Do not advance the sheath while the graft is still inside the sheath. Doing so may cause the barbs to perforate the introducer sheath.

## 3 UNSHEATHE THE PROXIMAL COMPONENT

While you constantly monitor the graft position, withdraw the sheath until the graft is fully expanded and the valve assembly with the Captor sleeve docks with the black gripper.

## 4 RELEASE THE PROXIMAL COMPONENT

Hold the black gripper and loosen the black safety-lock knob on the blue rotating handle (turn in the direction of the arrows). Turn the blue rotating handle following the directional arrow next to label 1 until a stop is felt. The stop indicates that the uncovered stent and proximal end of the graft have opened and the distal attachment to the introducer has been released.

## 5 REMOVE THE INTRODUCTION SYSTEM FOR THE PROXIMAL COMPONENT

Remove the introduction system entirely, leaving the wire guide positioned in the graft.

## 6 POSITION THE DISTAL COMPONENT

Introduce the hydrated introduction system until the desired graft position has been achieved. Ensure that there is a minimum overlap of 3 stents.

## 7 UNSHEATHE THE DISTAL COMPONENT

Stabilise the gray postioner and withdraw the sheath until the Captor sleeve docks with the telescoping black gripper.

## Deployment overview (continued)

### 8 RELEASE THE DISTAL COMPONENT

Use the **1-2-3** deployment sequence.

1. To release the distal attachment, hold the black sliding gripper and loosen the black safety-lock knob on the blue rotating handle (turn the safety lock in the direction of the arrows). Turn the blue rotating handle following the directional arrow next to **label 1** until a stop is felt.
2. Turn the gray safety-lock knob indicated by **label 2** on the black sliding gripper (turn the safety lock in the direction of the arrows). To release the distal bare stent, stabilise the introduction system and slide the black sliding gripper over the gray tube and outer sheath in a distal direction until it locks automatically into position next to the blue rotating handle (the release window on the blue rotating handle next to **label 3** will turn green).
3. Turn the blue rotating handle in the direction of the arrow (**label 3**) until a stop is felt and the proximal end of the graft opens.

### 9 OPTIONAL: MOLDING BALLOON

Advance the molding balloon over the wire guide and through the hemostatic valve of the main body introduction system to the level of the proximal fixation seal site. Maintain proper sheath positioning.

Tighten the Captor Hemostatic Valve around the molding balloon by turning it clockwise with gentle pressure.

**Caution:** Do not inflate the balloon in the vessel outside of the graft.

Expand the molding balloon with diluted contrast media (as directed by the manufacturer) in the area of the proximal covered stent, starting proximally and working in the distal direction.






Expect  
disease-specific  
solutions for  
type B dissections.

# Zenith<sup>®</sup> Dissection

ENDOVASCULAR SYSTEM

[back](#)

# Indications for use

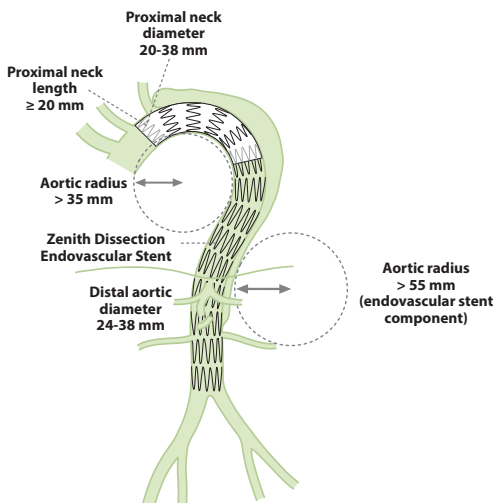

Indications for use	Patients with symptomatic aortic dissection distal to the left subclavian artery having vascular morphology suitable for endovascular repair.		
Length	Dissection stent lengths 82, 123, 164 mm used in combination with the sealing stent graft TX2 Proximal Component can potentially allow treatment of the entire descending thoracic aorta and the abdominal aorta.		
Aortic fixation site diameter	Dissection grafts: 20-38 mm (measured outer wall to outer wall) Dissection stents: 24-38 mm (measured outer wall to outer wall)		
Angulation/curvature	<ul style="list-style-type: none"> <li>• Aortic radius of <math>&gt; 35</math> degrees (dissection graft)</li> <li>• Radius of curvature <math>&gt; 55</math> mm along the length of the aorta that is intended to be treated (dissection stent)</li> <li>• Localized angulation <math>&gt; 35</math> degrees (dissection stent)</li> </ul>		
Access	Adequate femoral/iliac access compatible with the required introduction systems		
Introducer diameters	22-34 mm grafts: ID 20 Fr (6.7 mm) OD 7.7 mm	36-42 mm grafts: ID 22 Fr (7.3 mm) OD 8.5 mm	36, 46 mm stents: ID 16 Fr (5.3 mm) OD 6.5 mm
Contraindications	<ul style="list-style-type: none"> <li>• Patients with known sensitivities or allergies to stainless steel, polyester, nitinol, polypropylene, or gold</li> <li>• Patients with a systemic infection who may be at increased risk of endovascular stent/graft infection</li> </ul>		

# Zenith® TX2® Dissection Endovascular Graft with Pro-Form® straight components

Order Number	Reference Part Number	Component Type	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>						
G24249	ZDEG-P-22-79-PF	P	20	22	79	20 (6.7)/7.7
G24250	ZDEG-P-22-117-PF	P	20	22	117	20 (6.7)/7.7
<b>24 mm Diameter</b>						
G24251	ZDEG-P-24-79-PF	P	21	24	79	20 (6.7)/7.7
G24253	ZDEG-P-24-117-PF	P	21	24	117	20 (6.7)/7.7
<b>26 mm Diameter</b>						
G24255	ZDEG-P-26-79-PF	P	22-23	26	79	20 (6.7)/7.7
G24257	ZDEG-P-26-136-PF	P	22-23	26	136	20 (6.7)/7.7
<b>28 mm Diameter</b>						
G24260	ZDEG-P-28-82-PF	P	24	28	82	20 (6.7)/7.7
G24262	ZDEG-P-28-142-PF	P	24	28	142	20 (6.7)/7.7
G24265	ZDEG-P-28-202-PF	P	24	28	202	20 (6.7)/7.7
<b>30 mm Diameter</b>						
G24267	ZDEG-P-30-82-PF	P	25-27	30	82	20 (6.7)/7.7
G24269	ZDEG-P-30-142-PF	P	25-27	30	142	20 (6.7)/7.7
G24271	ZDEG-P-30-202-PF	P	25-27	30	202	20 (6.7)/7.7
<b>32 mm Diameter</b>						
G24272	ZDEG-P-32-82-PF	P	28-29	32	82	20 (6.7)/7.7
G24275	ZDEG-P-32-142-PF	P	28-29	32	142	20 (6.7)/7.7
G24276	ZDEG-P-32-202-PF	P	28-29	32	202	20 (6.7)/7.7
<b>34 mm Diameter</b>						
G24277	ZDEG-P-34-79-PF	P	30	34	79	20 (6.7)/7.7
G24278	ZDEG-P-34-154-PF	P	30	34	154	20 (6.7)/7.7
G24279	ZDEG-P-34-204-PF	P	30	34	204	20 (6.7)/7.7

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Zenith TX2 Dissection Endovascular Graft with Pro-Form straight components (continued)


Order Number	Reference Part Number	Component Type	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>36 mm Diameter</b>						
G24282	ZDEG-P-36-79-PF	P	31-32	36	79	22 (7.3)/8.5
G24283	ZDEG-P-36-154-PF	P	31-32	36	154	22 (7.3)/8.5
G24284	ZDEG-P-36-204-PF	P	31-32	36	204	22 (7.3)/8.5
<b>38 mm Diameter</b>						
G24285	ZDEG-P-38-79-PF	P	33-34	38	79	22 (7.3)/8.5
G24286	ZDEG-P-38-154-PF	P	33-34	38	154	22 (7.3)/8.5
G24287	ZDEG-P-38-204-PF	P	33-34	38	204	22 (7.3)/8.5
<b>40 mm Diameter</b>						
G24288	ZDEG-P-40-83-PF	P	35-36	40	83	22 (7.3)/8.5
G24289	ZDEG-P-40-164-PF	P	35-36	40	164	22 (7.3)/8.5
G24290	ZDEG-P-40-218-PF	P	35-36	40	218	22 (7.3)/8.5
<b>42 mm Diameter</b>						
G24291	ZDEG-P-42-83-PF	P	37-38	42	83	22 (7.3)/8.5
G24252	ZDEG-P-42-164-PF	P	37-38	42	164	22 (7.3)/8.5
G24292	ZDEG-P-42-218-PF	P	37-38	42	218	22 (7.3)/8.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


## Z-Trak Plus® Introduction System for straight components

22-34 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36-42 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



# Zenith TX2 Dissection Endovascular Graft with Pro-Form straight components

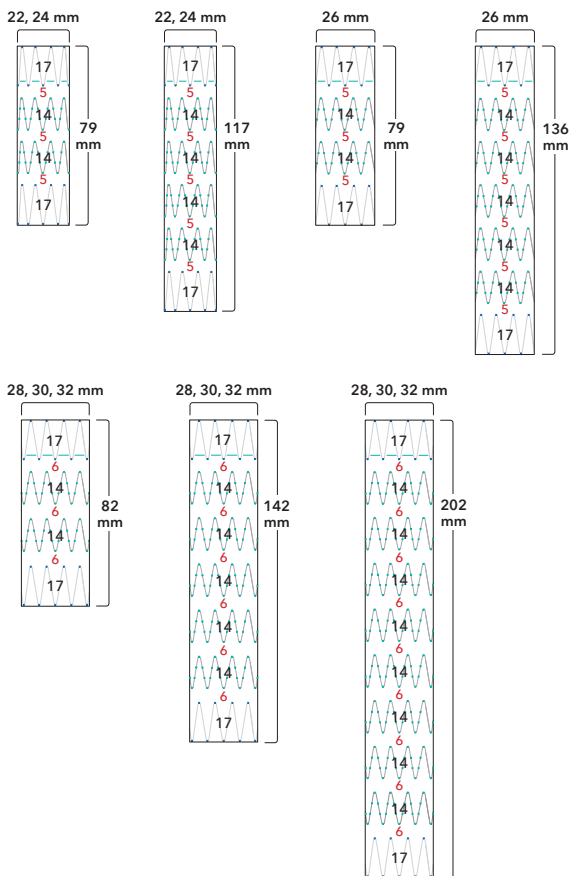


ZDEG-P-XX-YYY-PF

ZDEG-P-(diameter)-(length)-PF


**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

# Zenith TX2 Dissection Endovascular Graft with Pro-Form straight components (continued)


34, 36, 38 mm




34, 36, 38 mm




34, 36, 38 mm




40, 42 mm



40, 42 mm



40, 42 mm



# Zenith TX2 Dissection Endovascular Graft with Pro-Form 4 mm tapered components


Order Number	Reference Part Number	Component Type	Aortic Vessel OD mm	Proximal Diameter mm	Distal Diameter mm	Length mm	Introducer Sheath ID/OD Fr(mm)/mm
<b>32/28 mm Diameter</b>							
G24254	ZDEG-PT-32-162-PF	PT	28-29	32	28	162	20(6.7)/7.7
G24256	ZDEG-PT-32-202-PF	PT	28-29	32	28	202	20(6.7)/7.7
<b>34/30 mm Diameter</b>							
G24258	ZDEG-PT-34-159-PF	PT	30	34	30	159	20(6.7)/7.7
G24259	ZDEG-PT-34-199-PF	PT	30	34	30	199	20(6.7)/7.7
<b>36/32 mm Diameter</b>							
G24261	ZDEG-PT-36-159-PF	PT	31-32	36	32	159	22(7.3)/8.5
G24263	ZDEG-PT-36-199-PF	PT	31-32	36	32	199	22(7.3)/8.5
<b>38/34 mm Diameter</b>							
G24264	ZDEG-PT-38-154-PF	PT	33-34	38	34	154	22(7.3)/8.5
G24266	ZDEG-PT-38-204-PF	PT	33-34	38	34	204	22(7.3)/8.5
<b>40/36 mm Diameter</b>							
G24268	ZDEG-PT-40-160-PF	PT	35-36	40	36	160	22(7.3)/8.5
G24270	ZDEG-PT-40-210-PF	PT	35-36	40	36	210	22(7.3)/8.5
<b>42/38 mm Diameter</b>							
G24273	ZDEG-PT-42-160-PF	PT	37-38	42	38	160	22(7.3)/8.5
G24274	ZDEG-PT-42-210-PF	PT	37-38	42	38	210	22(7.3)/8.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


## Z-Trak Plus Introduction System for 4 mm tapered components

32–34 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36–42 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



# Zenith TX2 Dissection Endovascular Graft with Pro-Form 4 mm tapered components

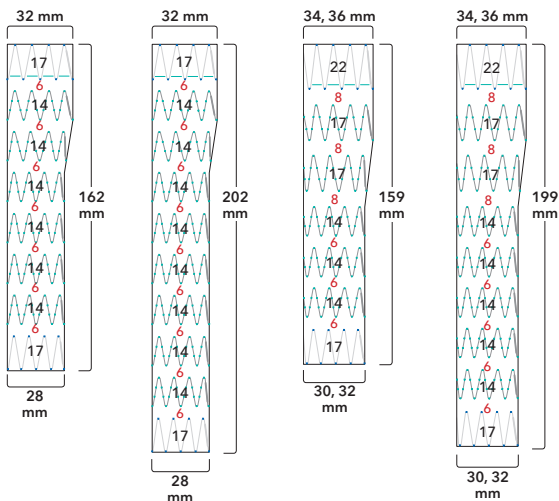

ZDEG-PT-XX-YYY-PF


ZDEG-PT-(proximal diameter)-(length)-PF

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.



# Zenith TX2 Dissection Endovascular Graft with Pro-Form 4 mm tapered components

(continued)



# Zenith TX2 Dissection Endovascular Graft with Pro-Form 8 mm tapered components


Order Number	Reference Part Number	Component Type	Aortic Vessel OD mm	Proximal Diameter mm	Distal Diameter mm	Length mm	Introducer Sheath ID/OD Fr(mm)/mm
<b>32/24 mm Diameter</b>							
G23172	ZDEG-PT-32-24-158-PF	PT	28-29	32	24	158	20 (6.7)/7.7
G23173	ZDEG-PT-32-24-196-PF	PT	28-29	32	24	196	20 (6.7)/7.7
<b>34/26 mm Diameter</b>							
G23174	ZDEG-PT-34-26-156-PF	PT	30	34	26	156	20 (6.7)/7.7
G23175	ZDEG-PT-34-26-194-PF	PT	30	34	26	194	20 (6.7)/7.7
<b>36/28 mm Diameter</b>							
G23176	ZDEG-PT-36-28-159-PF	PT	31-32	36	28	159	22 (7.3)/8.5
G23177	ZDEG-PT-36-28-199-PF	PT	31-32	36	28	199	22 (7.3)/8.5
<b>38/30 mm Diameter</b>							
G23178	ZDEG-PT-38-30-159-PF	PT	33-34	38	30	159	22 (7.3)/8.5
G23179	ZDEG-PT-38-30-199-PF	PT	33-34	38	30	199	22 (7.3)/8.5
<b>40/32 mm Diameter</b>							
G23180	ZDEG-PT-40-32-165-PF	PT	35-36	40	32	165	22 (7.3)/8.5
G23181	ZDEG-PT-40-32-205-PF	PT	35-36	40	32	205	22 (7.3)/8.5
<b>42/34 mm Diameter</b>							
G23182	ZDEG-PT-42-34-160-PF	PT	37-38	42	34	160	22 (7.3)/8.5
G23183	ZDEG-PT-42-34-210-PF	PT	37-38	42	34	210	22 (7.3)/8.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


## Z-Trak Plus Introduction System for 8 mm tapered component

32–34 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36–42 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



# Zenith TX2 Dissection Endovascular Graft with Pro-Form 8 mm tapered components

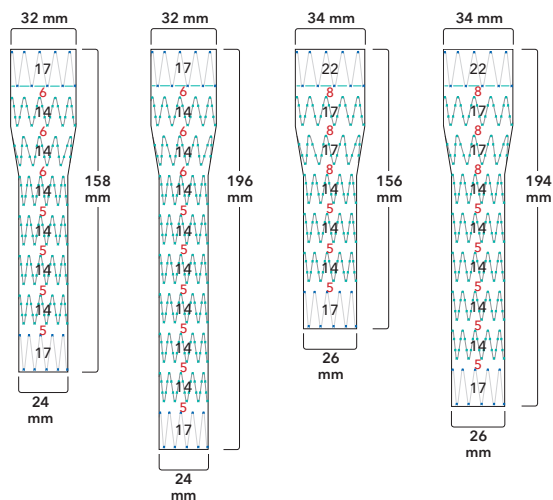


ZDEG-PT-XX-YY-ZZZ-PF

ZDEG-PT-(proximal diameter)-(distal diameter)-(length)-PF

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

# Zenith TX2 Dissection Endovascular Graft with Pro-Form 8 mm tapered components

(continued)

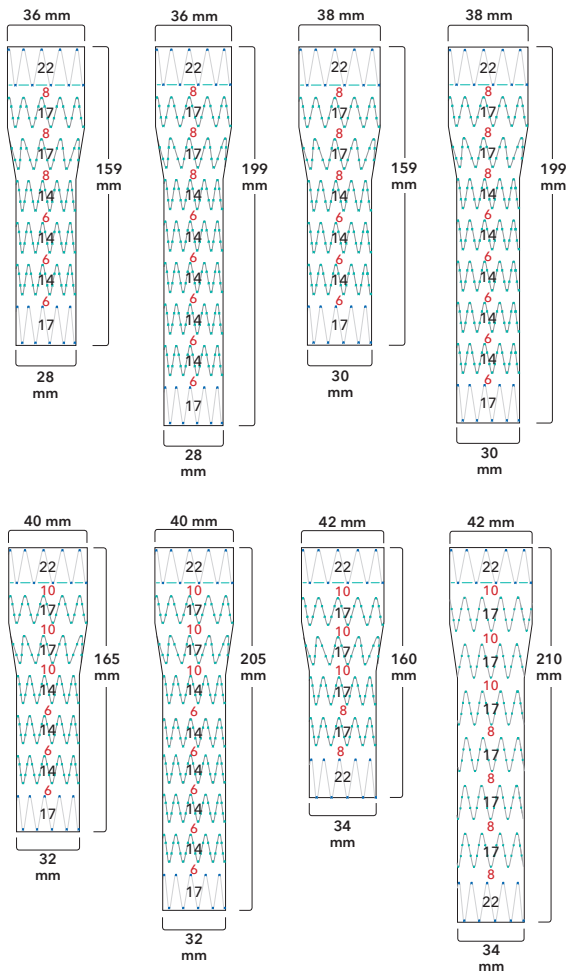


# Endovascular stents

Order Number	Reference Part Number	Aortic Vessel OD mm	Diameter mm	Length mm	Stents	Introducer Sheath ID/OD Fr(mm)/mm
<b>36 mm Diameter</b>						
G23615	GZSD-36-82-2	24-30	36	82	4	16 (5.3)/6.5
G23616	GZSD-36-123-2	24-30	36	123	6	16 (5.3)/6.5
G23617	GZSD-36-164-2	24-30	36	164	8	16 (5.3)/6.5
<b>46 mm Diameter</b>						
G23618	GZSD-46-82-2	31-38	46	82	4	16 (5.3)/6.5
G23619	GZSD-46-123-2	31-38	46	123	6	16 (5.3)/6.5
G23620	GZSD-46-164-2	31-38	46	164	8	16 (5.3)/6.5


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


## H&L-B One-Shot™ Introduction System for dissection stents

16 Fr (5.3 mm) ID/6.5 mm OD



# Endovascular stents






Select immediate options for acute treatment.

# Zenith<sup>®</sup> t-Branch<sup>®</sup>

THORACOABDOMINAL ENDOVASCULAR GRAFT

[back](#)

## Indications for use



### Indications for use

The Zenith t-Branch Thoracoabdominal Endovascular Graft is indicated for the endovascular treatment of high-risk patients with thoracoabdominal aneurysms who are not amenable to open surgical repair. The patients must have morphology suitable for endovascular repair, including:

- Adequate iliac/femoral access compatible with an 8.5 OD (22 Fr) introduction system,
- Nonaneurysmal thoracic aorta fixation segment proximal to the aneurysm:
  - With an angle of less than 90 degrees relative to the long axis of the aneurysm
  - With a length of at least 25 mm, (50 mm of wall contact is preferred)
  - With a diameter measured outer wall to outer wall of no greater than 30 mm and no less than 24 mm
- Alternatively, the Zenith t-Branch graft may be attached to a pre-existing endovascular graft such as the Zenith TX2 TAA Endovascular Graft.
- Visceral vessel anatomy compatible with Zenith t-Branch, specifically:
  - Four indispensable arteries from the abdominal viscera
  - All target arteries to be accessible from an antegrade approach
  - Celiac and superior mesenteric artery (SMA) to be 6 mm to 10 mm in diameter
  - Renal arteries to be 4 mm to 8 mm in diameter
  - The distance between each cuff and the corresponding arterial orifice is less than 50 mm
  - The line between the cuff and the arterial orifice as projected onto the vessel wall deviates by no more than 45 degrees from the long axis of the aorta.

### Length

Nonaneurysmal thoracic aorta fixation segment proximal to the aneurysm  $\geq 25$  mm (50 mm of wall contact is preferred)

### Aortic fixation site diameter

24-30 mm (measured outer wall to outer wall)

### Angulation/ Curvature

- An angle  $< 90$  degrees relative to the long axis of the aneurysm



## Indications for use (continued)

<b>Access</b>	Adequate iliac/femoral access compatible with an 8.5 OD (22 Fr) introduction system	
<b>Introducer diameters</b>	ID 22 Fr (7.3 mm) OD 8.5 mm	
<b>Contraindications</b>	<ul style="list-style-type: none"><li>• Patients with known sensitivities or allergies to stainless steel, nitinol, polyester, solder (tin, silver), polypropylene, urethane, or gold</li><li>• Patients with a systemic infection who may be at increased risk of endovascular stent infection</li></ul>	


# Thoracoabdominal (TAAA) endovascular graft

Order Number	Reference Part Number	Aortic Vessel OD mm	Proximal Diameter mm	Distal Diameter mm	Body Length mm	Introducer Sheath ID/OD Fr (mm)/mm
G55513	TBRANCH-34-18-202	24-30	34	18	202	22 (7.3)/8.5


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## H&L-B One-Shot™ Introduction System for t-Branch graft

22 Fr (7.3 mm) ID/8.5 mm OD



# Thoracoabdominal (TAAA) endovascular graft



## TBRANCH-34-18-202

TBRANCH-(proximal diameter)-(distal diameter)-(body length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.


# Universal distal body grafts

Order Number	Reference Part Number	Proximal Diameter mm	Distal Body Length mm	Introducer Sheath ID/OD Fr (mm)/mm
G55563	UNIBODY-22-81	22	81	20 (6.7)/7.7
G55564	UNIBODY-22-98	22	98	20 (6.7)/7.7
G55565	UNIBODY-22-115	22	115	20 (6.7)/7.7
G55566	UNIBODY-22-132	22	132	20 (6.7)/7.7


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## H&L-B One-Shot Introduction System for universal distal body grafts

20 Fr (6.7 mm) ID/7.7 mm OD



# Universal distal body grafts



UNIBODY-XX-YYY


UNIBODY-(proximal diameter)-(distal body length)

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

**Note:** Universal distal body is compatible with Zenith Spiral-Z<sup>®</sup> legs.

# Zenith® TX2® TAA Endovascular Graft with Pro-Form®

Compatible with Zenith® t-Branch™ Thoracoabdominal Endovascular Graft



Zenith t-Branch TAAA

Prox. 10 mm tpr.


# Zenith TX2 TAA Endovascular Graft with Pro-Form proximal 10 mm tapered components

Order Number	Reference Part Number	Component Type	Aortic Vessel OD mm	Proximal/ Distal Diameter mm	Length mm	Introducer Sheath Fr (mm)/mm
<b>38 mm Diameter</b>						
G23609	ZTEG-2PT-38-28-159-PF	2PT	33-34	38/28	159	22 (7.3)/8.5
G23610	ZTEG-2PT-38-28-199-PF	2PT	33-34	38/28	199	22 (7.3)/8.5
<b>40 mm Diameter</b>						
G23611	ZTEG-2PT-40-30-165-PF	2PT	35-36	40/30	165	22 (7.3)/8.5
G23612	ZTEG-2PT-40-30-205-PF	2PT	35-36	40/30	205	22 (7.3)/8.5
<b>42 mm Diameter</b>						
G23613	ZTEG-2PT-42-32-165-PF	2PT	37-38	42/32	165	22 (7.3)/8.5
G23614	ZTEG-2PT-42-32-205-PF	2PT	37-38	42/32	205	22 (7.3)/8.5


Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Z-Trak Plus Introduction System for proximal 10 mm tapered components

38-42 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



# Zenith TX2 TAA Endovascular Graft with Pro-Form proximal 10 mm tapered components

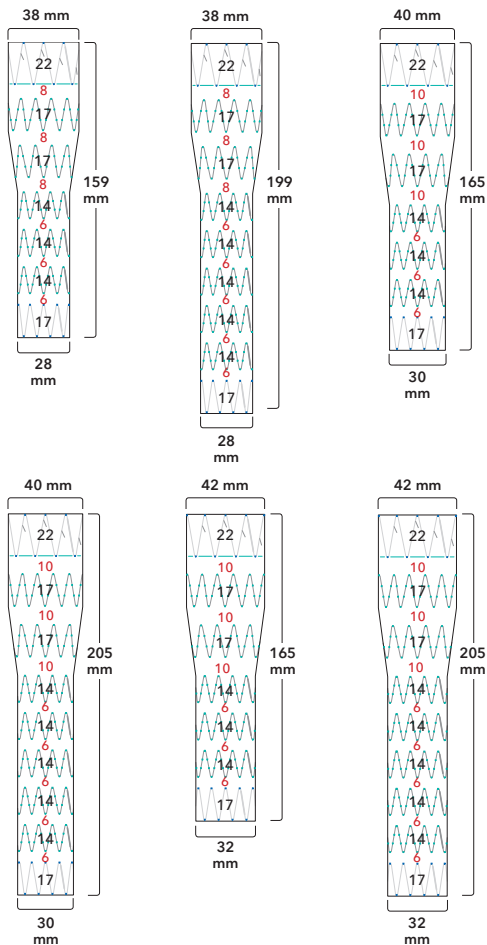

ZTEG-2PT-XX-YYY-PF

ZTEG-2PT-(proximal diameter)-(length)-PF

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

**Note:** Part numbers indicated are compatible with Zenith t-Branch TAAA.



# Zenith TX2 TAA Endovascular Graft with Pro-Form proximal extensions


Order Number	Reference Part Number	Component Type	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>34 mm Diameter</b>						
G52652	TBE-34-77-PF	TBE	30	34	77	20 (6.7)/7.7
<b>36 mm Diameter</b>						
G52653	TBE-36-77-PF	TBE	31-32	36	77	22 (7.3)/8.5
<b>38 mm Diameter</b>						
G52654	TBE-38-77-PF	TBE	33-34	38	77	22 (7.3)/8.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


## Z-Trak Plus Introduction System for proximal extensions

34 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD

36-38 mm grafts: 22 Fr (7.3 mm) ID/8.5 mm OD



34, 36, 38 mm



TBE-XX-YY-PF

TBE-(diameter)-(length)-PF

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.

**Note:** Part numbers indicated are compatible with Zenith t-Branch TAAA.



# Zenith TX2 TAA Endovascular Graft with Pro-Form distal extensions

Order Number	Reference Part Number	Component Type	Aortic Vessel OD mm	Diameter mm	Length mm	Introducer Sheath ID/OD Fr (mm)/mm
<b>22 mm Diameter</b>						
<b>G52635</b>	<b>ESBE-22-80-T-PF</b>	ESBE	20	22	80	20 (6.7)/7.7

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Z-Trak Plus Introduction System for distal extensions

22 mm grafts: 20 Fr (6.7 mm) ID/7.7 mm OD




**ESBE-XX-YY-T-PF**

**ESBE-(diameter)-(length)-T-PF**

**Note:** All measurements are in millimetres. The black numbers on the illustrations indicate stent lengths. The red numbers indicate gap lengths. Gap lengths are approximate.


**Note:** Part numbers indicated are compatible with Zenith t-Branch TAAA.



## Accessories for endovascular procedures

[back](#)

# Coda® Balloon Catheter




Order Number	Reference Part Number	Catheter Diameter/Length Fr/cm	Recommended Introducer Fr
G03831	CODA-2-9.0-35-120-32	9/120	12
G23773	CODA-2-10.0-35-140-46*	10/140	14

Accepts Wire Guide Diameter inch	Balloon Maximum Inflated Diameter mm	Balloon Maximum Inflation Volume mL
.035	32	30
.035	46	60

Some products or part numbers may not be available in all markets. Contact your

\*The 46 mm Coda Balloon Catheter should not be used in vessels < 24 mm in diameter or for expansion of vascular prostheses within iliac or other nonaortic vessels.

# Lunderquist® Extra-Stiff Wire Guide




Order Number	Reference Part Number	Diameter inch	Length cm	Flexible Tip Length cm	Tip Curve Radius mm	Coil Length cm
<b>Straight Exchange – PTFE-Coated Stainless Steel</b>						
G31453	TSMG-35-260-LES	.035	260	4	straight	15
G45352	TSMG-35-300-LES	.035	300	4	straight	15
<b>Curved Exchange – PTFE-Coated Stainless Steel</b>						
G45353	TSCMG-35-260-7-LES	.035	260	4	7.5	15
G45407	TSCMG-35-300-7-LES	.035	300	4	7.5	15

Order Number	Reference Part Number	Diameter inch	Length cm	Flexible Tip Length cm	Primary/Secondary Curve Radius mm	Coil Length cm
<b>Double Curved Exchange – PTFE-Coated Stainless Steel</b>						
G45208	TSCMG-35-260-LESDC	.035	260	4	75/15	15
G45408	TSCMG-35-300-LESDC	.035	300	4	75/15	15
<b>Extended Double Curved Exchange – PTFE-Coated Stainless Steel</b>						
G53967	TSCMG-35-260-E-LESDC	.035	260	4	55/15	15
G53971	TSCMG-35-300-E-LESDC	.035	300	4	55/15	15

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


## Indy OTW™ Vascular Retriever



Order Number	Reference Part Number	Sheath OD Fr	Accepts Wire Guide Diameter inch	Sheath Length cm	Basket Diameter mm
<b>G51835</b>	<b>INDY-8.0-35-55-40</b>	8.0	.035	55	40
<b>G51836</b>	<b>INDY-8.0-35-100-40</b>	8.0	.035	100	40

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Van Schie Beacon® Tip Seeking Catheter



Order Number	Reference Part Number	Fr	Accepts Wire Guide Diameter inch	Length cm
G31410	HNBR5.0-35-40-P-NS-VANSCHIE1	5.0	.035	40
G31409	HNBR5.0-35-40-P-NS-VANSCHIE2	5.0	.035	40
G31408	HNBR5.0-35-40-P-NS-VANSCHIE3	5.0	.035	40
G13795	HNBR5.0-35-65-P-NS-VANSCHIE1	5.0	.035	65
G13794	HNBR5.0-35-65-P-NS-VANSCHIE2	5.0	.035	65
G13792	HNBR5.0-35-65-P-NS-VANSCHIE3	5.0	.035	65
G13783	HNBR5.0-35-65-P-NS-VANSCHIE4	5.0	.035	65
G13793	HNBR5.0-35-65-P-NS-VANSCHIE5	5.0	.035	65
G35733	HNBR5.0-35-125-P-NS-VANSCHIE1	5.0	.035	125
G35734	HNBR5.0-35-125-P-NS-VANSCHIE2	5.0	.035	125
G35735	HNBR5.0-35-125-P-NS-VANSCHIE3	5.0	.035	125
G35736	HNBR5.0-35-125-P-NS-VANSCHIE4	5.0	.035	125
G35737	HNBR5.0-35-125-P-NS-VANSCHIE5	5.0	.035	125

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Endovascular Dilator Set



Order Number	Reference Part Number	Accepts Wire Guide Diameter inch	Fr	Length cm	Hydrophilic Coated
G52833	JCDS-14-EDS-HC	.035	14.0	45	yes
G52834	JCDS-1618-EDS-HC	.035	16.0, 18.0	45	yes
G52835	JCDS-2022-EDS-HC	.035	20.0, 22.0	45	yes
G52836	JCDS-2426-EDS-HC	.035	24.0, 26.0	45	yes

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.



# Aurous™ Centimetre Sizing Catheter



Order Number	Reference Part Number	Fr	Accepts Wire Guide Diameter inch	Length cm	Side-ports	Number of Bands/ Placement Interval cm
<b>Pigtail</b>						
G31215	NR5.0-35-70-P-10S-PIG-CSC-20	5.0	.035	70	10	21/1
G31216	NR5.0-35-100-P-10S-PIG-CSC-20	5.0	.035	100	10	21/1
<b>Straight</b>						
G31213	NR5.0-35-70-P-10S-0-CSC-20	5.0	.035	70	10	21/1
G31214	NR5.0-35-100-P-10S-0-CSC-20	5.0	.035	100	10	21/1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


# Beacon® Tip Torcon NB® Advantage Catheter



Order Number	Reference Part Number	Fr	Accepts Wire Guide Diameter inch	Length cm	Tip Configuration
G08444	HNBR5.0-35-65-P-NS-RIM	5.0	.035	65	RIM
G08442	HNBR5.0-35-65-P-NS-C2	5.0	.035	65	C2
G08443	HNBR5.0-35-65-P-NS-C3	5.0	.035	65	C3
G09548	HNBR5.0-38-40-P-NS-KMP	5.0	.038	40	KMP
G11377	HNBR5.0-38-65-P-NS-TEGT	5.0	.038	65	TEGT
G11209	HNBR5.0-38-80-P-NS-VS	5.0	.038	80	VS
G35974	HNBR5.0-35-125-P-NS-VS1	5.0	.035	125	VS1
G31970	HNBR5.0-35-125-P-NS-C-PS	5.0	.035	125	C (Curly Q)

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Beacon® Tip Royal Flush® Plus High-Flow Catheter



Order Number	Reference Part Number	Fr	Accepts Wire Guide Diameter inch	Length cm	Tip Configuration	Spiraled Sideports
<b>Straight</b>						
G09411	HNR5.0-35-70-P-10S-0	5.0	.035	70	straight	10
G11270	HNR5.0-38-70-P-10S-0	5.0	.038	70	straight	10
G09697	HNR5.0-35-100-P-10S-0	5.0	.035	100	straight	10
G11267	HNR5.0-38-100-P-10S-0	5.0	.038	100	straight	10
<b>Pigtail</b>						
Standard Pigtail						
G08832	HNR5.0-35-70-P-10S-PIG	5.0	.035	70	PIG	10
G11272	HNR5.0-38-70-P-10S-PIG	5.0	.038	70	PIG	10
G09059	HNR5.0-35-100-P-10S-PIG	5.0	.035	100	PIG	10
G09285	HNR5.0-38-100-P-10S-PIG	5.0	.038	100	PIG	10
Centra-Flo™ Pigtail						
G11262	HNR5.0-35-70-P-10S-CFP	5.0	.035	70	CFP	10
G11268	HNR5.0-38-100-P-10S-CFP	5.0	.038	100	CFP	10
<b>Verrill Contralateral Flush</b>						
G12129	HNR5.0-35-65-P-8S-VCF	5.0	.035	65	VCF	8

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Nester® Embolisation Coils



Order Number	Reference Part Number	Recommended Catheter ID and End Hole Diameter inch	Extended Embolus Length cm	Coiled Embolus Diameter mm	Approximate Number of Loops
<b>.035 Inch Extended Coil Diameter</b>					
G26993	MWCE-35-14-4-NESTER	.035	14	4	11.1
G26994	MWCE-35-14-6-NESTER	.035	14	6	7.4
G26995	MWCE-35-14-8-NESTER	.035	14	8	5.6
G26991	MWCE-35-14-10-NESTER	.035	14	10	4.5
G26992	MWCE-35-14-12-NESTER	.035	14	12	3.7

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.


# Tornado® Embolisation Coils



Order Number	Reference Part Number	Recommended Catheter ID and End Hole Diameter inch	Extended Embolus Length cm	Coiled Embolus Tapering Diameter mm
<b>.035 Inch Extended Coil Diameter</b>				
G10415	MWCE-35-5/3-TORNADO	.035	4.1	5-3
G10416	MWCE-35-6/3-TORNADO	.035	5.8	6-3
G10417	MWCE-35-7/3-TORNADO	.035	8	7-3
G10411	MWCE-35-8/4-TORNADO	.035	8	8-4
G10412	MWCE-35-8/5-TORNADO	.035	8.2	8-5
G10413	MWCE-35-10/5-TORNADO	.035	12.5	10-5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Extra-Large Check-Flo® Performer™ Introducer




Order Number	Reference Part Number	Introducer* Fr	Accepts Wire Guide Diameter inch	Sheath Length cm	Dialator Length cm
G33060	XLCFW-14.0-38-30-ENDOSTENT	14.0	.038	30	46
G28990	XLCFW-16.0-38-30-ENDOSTENT	16.0	.038	30	46
G28991	XLCFW-16.0-38-55-ENDOSTENT	16.0	.038	55	71
G28992	XLCFW-18.0-38-30-ENDOSTENT	18.0	.038	30	46
G46788	XLCFW-20.0-38-25-ENDOSTENT	20.0	.038	25	41
G28993	XLCFW-20.0-38-30-ENDOSTENT	20.0	.038	30	46
G28994	XLCFW-20.0-38-40-ENDOSTENT	20.0	.038	40	56
G28995	XLCFW-20.0-38-55-ENDOSTENT	20.0	.038	55	71
G28996	XLCFW-22.0-38-30-ENDOSTENT	22.0	.038	30	46
G28997	XLCFW-22.0-38-40-ENDOSTENT	22.0	.038	40	56
G28998	XLCFW-24.0-38-30-ENDOSTENT	24.0	.038	30	46

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

\*Determine the maximum diameter of the instrument or catheter to be introduced to ensure its passage through the sheath.

# Flexor® Keller-Timmermans Introducer Set



Order Number	Reference Part Number	Introducer* Fr	Accepts Wire Guide Diameter inch	Sheath Length cm	Inner Diameter mm
<b>Straight Exchange</b>					
G49673	KSSW-20.0-38-65-0-KTI-HC	20.0	.038	65	6.88
G43897	KSSW-22.0-38-65-0-KTI-HC	22.0	.038	65	7.57
G43898	KSSW-24.0-38-65-0-KTI-HC	24.0	.038	65	8.18

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

\*Determine the maximum diameter of the instrument or catheter to be introduced to ensure its passage through the sheath.

# Flexor® Check-Flo® Introducers with Ansel Modification and High-Flex Dilator



Order Number	Reference Part Number	Introducer Fr	Sheath ID inch/mm	Accepts Wire Guide Diameter inch	Sheath Length cm	Tip Conf.*
G56229	KCFW-4.0-35-55-RB-HFANL0-HC	4.0	.059/1.5	.035	55	s
G56234	KCFW-4.0-35-55-RB-HFANL1-HC	4.0	.059/1.5	.035	55	m
G56219	KCFW-4.0-35-70-RB-HFANL0-HC	4.0	.059/1.5	.035	70	s
G56224	KCFW-4.0-35-70-RB-HFANL1-HC	4.0	.059/1.5	.035	70	m
G56230	KCFW-5.0-35-55-RB-HFANL0-HC	5.0	.074/1.9	.035	55	s
G56235	KCFW-5.0-35-55-RB-HFANL1-HC	5.0	.074/1.9	.035	55	m
G56220	KCFW-5.0-35-70-RB-HFANL0-HC	5.0	.074/1.9	.035	70	s
G56225	KCFW-5.0-35-70-RB-HFANL1-HC	5.0	.074/1.9	.035	70	m
G56231	KCFW-6.0-35-55-RB-HFANL0-HC	6.0	.087/2.2	.035	55	s
G56236	KCFW-6.0-35-55-RB-HFANL1-HC	6.0	.087/2.2	.035	55	m
G56221	KCFW-6.0-35-70-RB-HFANL0-HC	6.0	.087/2.2	.035	70	s
G56226	KCFW-6.0-35-70-RB-HFANL1-HC	6.0	.087/2.2	.035	70	m
G56232	KCFW-7.0-35-55-RB-HFANL0-HC	7.0	.100/2.5	.035	55	s
G49043	KCFW-7.0-35-55-RB-HFANL1-HC	7.0	.100/2.5	.035	55	m
G56222	KCFW-7.0-35-70-RB-HFANL0-HC	7.0	.100/2.5	.035	70	s
G56227	KCFW-7.0-35-70-RB-HFANL1-HC	7.0	.100/2.5	.035	70	m
G49044	KCFW-7.0-35-110-RB-HFANL1-HC	7.0	.100/2.5	.035	110	m
G56233	KCFW-8.0-35-55-RB-HFANL0-HC	8.0	.113/2.9	.035	55	s
G49045	KCFW-8.0-35-55-RB-HFANL1-HC	8.0	.113/2.9	.035	55	m
G56223	KCFW-8.0-35-70-RB-HFANL0-HC	8.0	.113/2.9	.035	70	s

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

\*Tip Configuration: s = straight, m = multipurpose

[back](#)




## Flexor® Check-Flo® Introducers with Ansel Modification and High-Flex Dilator



Order Number	Reference Part Number	Introducer Fr	Sheath ID inch/mm	Accepts Wire Guide Diameter inch	Sheath Length cm	Tip Conf.*
G56228	KCFW-8.0-35-70-RB-HFANL1-HC	8.0	.113/2.9	.035	70	m
G49046	KCFW-8.0-35-110-RB-HFANL1-HC	8.0	.113/2.9	.035	110	m
G56278	KCFW-10.0-35-45-RB-HFANL0-HC	10.0	.134/3.4	.035	45	s
G47700	KCFW-10.0-35-45-RB-HFANL1-HC	10.0	.134/3.4	.035	45	m
G56279	KCFW-12.0-35-45-RB-HFANL0-HC	12.0	.162/4.1	.035	45	s
G47701	KCFW-12.0-35-45-RB-HFANL1-HC	12.0	.162/4.1	.035	45	m

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Check-Flo® Performer® Introducer



Order Number	Reference Part Number	*Introducer Fr	Accepts Wire Guide Diameter inch	Wire Guide Tip Configuration	Sheath Length cm	Dilator Length cm
<b>Standard With Wire Guide</b>						
G07605	RCF-5.0-35-J	5.0	.035	J	13	20
G07376	RCF-6.0-35-J	6.0	.035	J	13	20
G07377	RCF-7.0-35-J	7.0	.035	J	13	20
G07487	RCF-5.0-38-J	5.0	.038	J	13	20
G07337	RCF-6.0-38-J	6.0	.038	J	13	20
G07338	RCF-7.0-38-J	7.0	.038	J	13	20
G07490	RCF-8.0-38-J	8.0	.038	J	13	20
<b>Standard Without Wire Guide</b>						
G07427	RCFW-5.0-35	5.0	.035	-	13	20
G07428	RCFW-5.0-38	5.0	.038	-	13	20
G07548	RCFW-5.5-38	5.5	.038	-	13	20
G07420	RCFW-6.0-38	6.0	.038	-	13	20
G07431	RCFW-7.0-38	7.0	.038	-	13	20
G07432	RCFW-8.0-38	8.0	.038	-	13	20
<b>Standard With Radiopaque Band Without Wire Guide</b>						
G08452	RCFW-5.0-35-RB	5.0	.035	-	13	20
G07919	RCFW-6.0-35-RB	6.0	.035	-	13	20
G09118	RCFW-7.0-35-RB	7.0	.035	-	13	20

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

\*Determine the maximum diameter of the instrument or catheter to be introduced to ensure its passage through the sheath.

[back](#)


# Amplatz Ultra Stiff Wire Guide



Order Number	Reference Part Number	Diameter inch	Length cm	Flexible Tip Length cm	Tip Curve Radius mm	Taper Length cm
<b>Straight Exchange</b>						
G19854	THSF-35-260-AUS2	.035	260	6.5	straight	13.5
<b>Curved Exchange</b>						
G20320	THSCF-35-260-3-AUS2	.035	260	6.5	3	13.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Roadrunner® UniGlide® Hydrophilic Wire Guide



Order Number	Reference Part Number	Diameter inch	Length cm	Tip Configuration
<b>Stiff Shaft</b>				
G56152	HPWS-35-150	.035	150	straight
G56153	HPWS-35-180	.035	180	straight
G56176	HPWAS-35-150	.035	150	angled
G56177	HPWAS-35-180	.035	180	angled

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Roadrunner® PC Hydrophilic Wire Guide



Order Number	Reference Part Number	Diameter inch	Length cm	Tip Configuration	Flexible Tip Length cm
<b>Nimble®</b> Short Taper, Flexible Shaft with Polyurethane-Coated Nitinol Core and AQ® Hydrophilic Coating					
G09607	RFSPC-35-145	.035	145	angled	3
G09608	RFSPC-35-180	.035	180	angled	3
<b>The Firm™</b> Short Taper, Flexible Shaft with Polyurethane-Coated Nitinol Core and AQ® Hydrophilic Coating					
G06979	RPC-35-145	.035	145	angled	3
G07518	RPC-35-180	.035	180	angled	3
G09105	RPC-35-260	.035	260	angled	3

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Percutaneous Entry Thinwall Needle—One-Part



Order Number	Reference Part Number	Accepts Wire Guide Diameter inch (mm)	gage	Length cm
G00272	SDN-18-5.0	.035/.038 (0.89/0.97)	18	5
G00166	SDN-18-7.0	.035/.038 (0.89/0.97)	18	7
G00273	SDN-18-9.0	.035/.038 (0.89/0.97)	18	9
G05399	SDN-19UT-5.0	.035/.038 (0.89/0.97)	19UT	5
G04876	SDN-19UT-7.0	.035/.038 (0.89/0.97)	19UT	7
G04893	SDN-19UT-9.0	.035/.038 (0.89/0.97)	19UT	9

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Rosen Curved Wire Guide



Order Number	Reference Part Number	Diameter inch	Length cm	Tip Curve Radius mm
<b>Curved – PTFE-Coated Stainless Steel</b>				
G01261	THSCF-35-145-1.5-ROSEN	.035	145	1.5
G01264	THSCF-35-180-1.5-ROSEN	.035	180	1.5
<b>Exchange, Curved – PTFE-Coated Stainless Steel</b>				
G01253	THSCF-35-260-1.5-ROSEN	.035	260	1.5

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.







## Endovascular graft procedure packs

[back](#)

# Zenith Alpha™ Abdominal Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
<b>G34907</b>	<b>ZAPP-A</b>	Pack consists of the components listed	
	RCFN-6.0-38-J	Check-Flo® Performer™ Introducer Set	2
	TSCF-35-180-3	Standard Wire Guide	1
	HWAS-35-180	HiWire® Hydrophilic Wire Guide	1
	NR5.0-35-100-P-10S-PIG-CSC-20	Aurous™ Centimetre	1
	TSCMG-35-260-7-LES	Lunderquist® Extra-Stiff Wire Guide	2
	HNBR5.0-35-65-P-NS-VANSCHIE2	Torcon NB® Advantage Van Schie Beacon® Tip Seeking Catheter	1
	HNBR5.0-35-65-P-NS-VANSCHIE5	Torcon NB Advantage Van Schie Beacon Tip Seeking Catheter	1
	CODA-2-9.0-35-120-32	Coda® Balloon Catheter	1

Some products or part numbers may not be available in all markets. Contact your

## Zenith AAA Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
<b>G50631</b>	<b>ESSK-AAA</b>	Pack consists of the components listed	
	TSCMG-35-260-7-LES	Lunderquist® Extra-Stiff Wire Guide	2
	CODA-2-9.0-35-120-32	Coda® Balloon Catheter	1
	HNBR5.0-35-65-P-NS-VANSCHIE2	Torcon NB® Advantage Van Schie Beacon® Tip Seeking Catheter	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Zenith® AAA Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
<b>G33036</b>	<b>ESSK-2</b>	Pack consists of the components listed	
	SDN-19UT-7.0	One-Part Percutaneous Entry Needle	2
	RCF-7.0-35-J	Check-Flo® Performer™ Introducer Set	2
	RFSPC-35-180	Roadrunner® PC Wire Guide, Nimble® Floppy	1
	TSCMG-35-260-7-LES	Lunderquist Extra-Stiff Wire Guide	2
	CODA-2-9.0-35-120-32	Coda® Balloon Catheter	1
	HNRS.0-35-100-P-10S-PIG	Beacon® Tip Royal Flush Plus Plus Catheter	1
	HNBR5.0-35-65-P-NS-VANSCHIE2	Torcon NB® Advantage Van Schie Beacon® Tip Seeking Catheter	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

# Zenith AAA Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
<b>G33037</b>	<b>ESSK-3</b>	Pack consists of the components listed	
	SDN-19UT-7.0	One-Part Percutaneous Entry Needle	2
	RCF-7.0-35-J	Check-Flo® Performer™ Introducer	2
	TSCF-35-145-3	Safe-T-J® Curved Fixed Core Wire Guide	1
	TSCMG-35-260-7-LES	Lunderquist Extra-Stiff Wire Guide	2
	HNR5.0-35-70-P-105-0	Royal Flush® Plus Straight Angiographic Catheter with Beacon Tip	1
	HNR5.0-35-100-P-105-PIG	Beacon® Tip Royal Flush Plus Plus Catheter	1
	NR5.0-35-100-P-105-PIG-CSC-20	Aurous™ Beacon Tip Sizing Catheter	1
	CODA-2-9.0-35-120-32	Coda® Balloon Catheter	1
	HNBR5.0-35-65-P-NS-VANSCHIE2	Torcon NB® Advantage Van Schie Beacon® Tip Seeking Catheter	1
	HNBR5.0-35-60-P-NS-BELL-1.5	Torcon NB Advantage Beacon Tip High-Flow Catheter	1
	HNBR5.0-35-65-P-NS-C2	Torcon NB Advantage Cobra Angiographic Catheter with Beacon Tip	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Zenith® Branch Iliac Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
G55527	ESSK-BRANCH	Pack consists of the components listed	
	THSCF-35-260-1.5-ROSEN	Safe-T-J® Rosen Catheter Exchange Wire Guide	1
	KCFW-7.0-35-55-RB-HFANL1-HC	Flexor® High-Flex Ansel Guiding Sheath	1
	KCFW-8.0-35-55-RB-HFANL1-HC	Flexor High-Flex Ansel Guiding Sheath	1
	KCFW-12.0-35-45-RB-HFANL1-HC	Flexor High-Flex Ansel Guiding Sheath	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Zenith® Fenestrated Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
G45702	ESSK-FEN	Pack consists of the components listed	
	XLCFW-20.0-38-30-ENDOSTENT	Extra-Large Check-Flo® Performer™ Introducer	1
	KCFW-7.0-35-55-RB-HFANL1-HC	Flexor® High-Flex Ansel Guiding Sheath	2
	THSCF-35-260-1.5-ROSEN	Safe-T-J® Rosen Catheter Exchange Wire Guide	2

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

**Note:** To support a Zenith Fenestrated case, you need to order both a Zenith AAA Endovascular Graft Procedure Pack and a Zenith Fenestrated Endovascular Graft Procedure Pack.

# Zenith® Alpha Thoracic Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
<b>G34908</b>	<b>ZAPP-T</b>	Pack consists of the components listed	
	RCFN-6.0-38-J	Check-Flo® Performer™ Introducer Set	1
	TSCF-35-180-3	Standard Wire Guide	1
	HWAS-35-180	HiWire® Hydrophilic Wire Guide	1
	NR5.0-35-100-P-10S-PIG-CSC-20	Aurous™ Centimetre Sizing Catheter	1
	TSCMG-35-300-LESDC	Lunderquist® Extra-Stiff Double Curved Wire Guide	1
	CODA-2-10.0-35-140-46	Coda® Balloon Catheter	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

## Zenith® TAA Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
<b>G39775</b>	<b>ESSK-T</b>	Pack consists of the components listed	
	<b>CODA-2-10.0-35-140-46</b>	Coda® Balloon Catheter	1
	<b>TSCMG-35-300-LESDC</b>	Lunderquist® Extra-Stiff Double Curved Wire Guide	1
	<b>RCFN-6.0-38-J</b>	Check-Flo® Performer™ Introducer Set	1
	<b>RFPC-35-180</b>	Roadrunner® PC Wire Guide, Nimble Floppy	1
	<b>NR5.0-35-100-P-10S-PIG-CSC-20</b>	Aurous™ Beacon® Tip Sizing Catheter	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.



# Zenith® t-Branch Endovascular Graft Procedure Pack

Order Number	Reference Part Number	Description	Qty
<b>G24065</b>	<b>ESSK-T-BRANCH</b>	Pack consists of the components listed	
	SDN-19UT-7.0	Vascular Access Needle	2
	RCF-7.0-35-J	Performer™ Introducer	3
	TSCF-35-260-3	Standard Wire Guide	1
	TSCMG-35-260-E-LESDC	Lunderquist® Extra-Stiff Extended Double Curve Wire Guide	1
	TSCMG-35-300-E-LESDC	Lunderquist Extra-Stiff Extended Double Curve Wire Guide	1
	THSF-35-260-AUS1	Amplatz Ultra-Stiff Support Wire Guide	2
	THSCF-35-260-1.5-ROSEN	Safe-T-J® Rosen Catheter Exchange Wire Guide	2
	RSTF-18-300	Roadrunner® Extra-Support Bare Mandril Wire Guide	1
	NR5.0-35-100-P-10S-PIG-CSC-20	Beacon® Tip Aorous Centimetre Vessel Sizing Catheter	1
	HNBR5.0-35-65-P-NS-VANSCHIE1	Torcon NB® Advantage Van Schie Beacon Tip Seeking Catheter	1
	HNBR5.0-35-65-P-NS-VANSCHIE2	Torcon NB Advantage Van Schie Beacon Tip Seeking Catheter	1
	HNBR5.0-35-65-P-NS-VANSCHIE3	Torcon NB Advantage Van Schie Beacon Tip Seeking Catheter	1
	HNBR5.0-38-100-P-NS-DAV	Beacon Tip Torcon NB Advantage Angiographic Catheter	1
	HNBR5.0-38-100-P-NS-H1	Beacon Tip Torcon NB Advantage Angiographic Catheter	1
	HNBR5.0-38-100-P-NS-MPA	Beacon Tip Torcon NB Advantage Angiographic Catheter	1
	HNBR5.0-38-100-P-NS-RIM	Beacon Tip Torcon NB Advantage Angiographic Catheter	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.

[back](#)

<b>Order Number</b>	<b>Reference Part Number</b>	<b>Description</b>	<b>Qty</b>
	KCFW-12.0-35-45-RB-HFANL1-HC	Flexor® High-Flex Ansel Guiding Sheath	1
	KCFW-10.0-38-80-RB	Flexor Guiding Sheath	1
	KCFW-8.0-38-70-RB-RAABE	Flexor Raabe Guiding Sheath	1
	CODA-2-10.0-35-140-46	Coda® Balloon Catheter	1

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Service for details.



